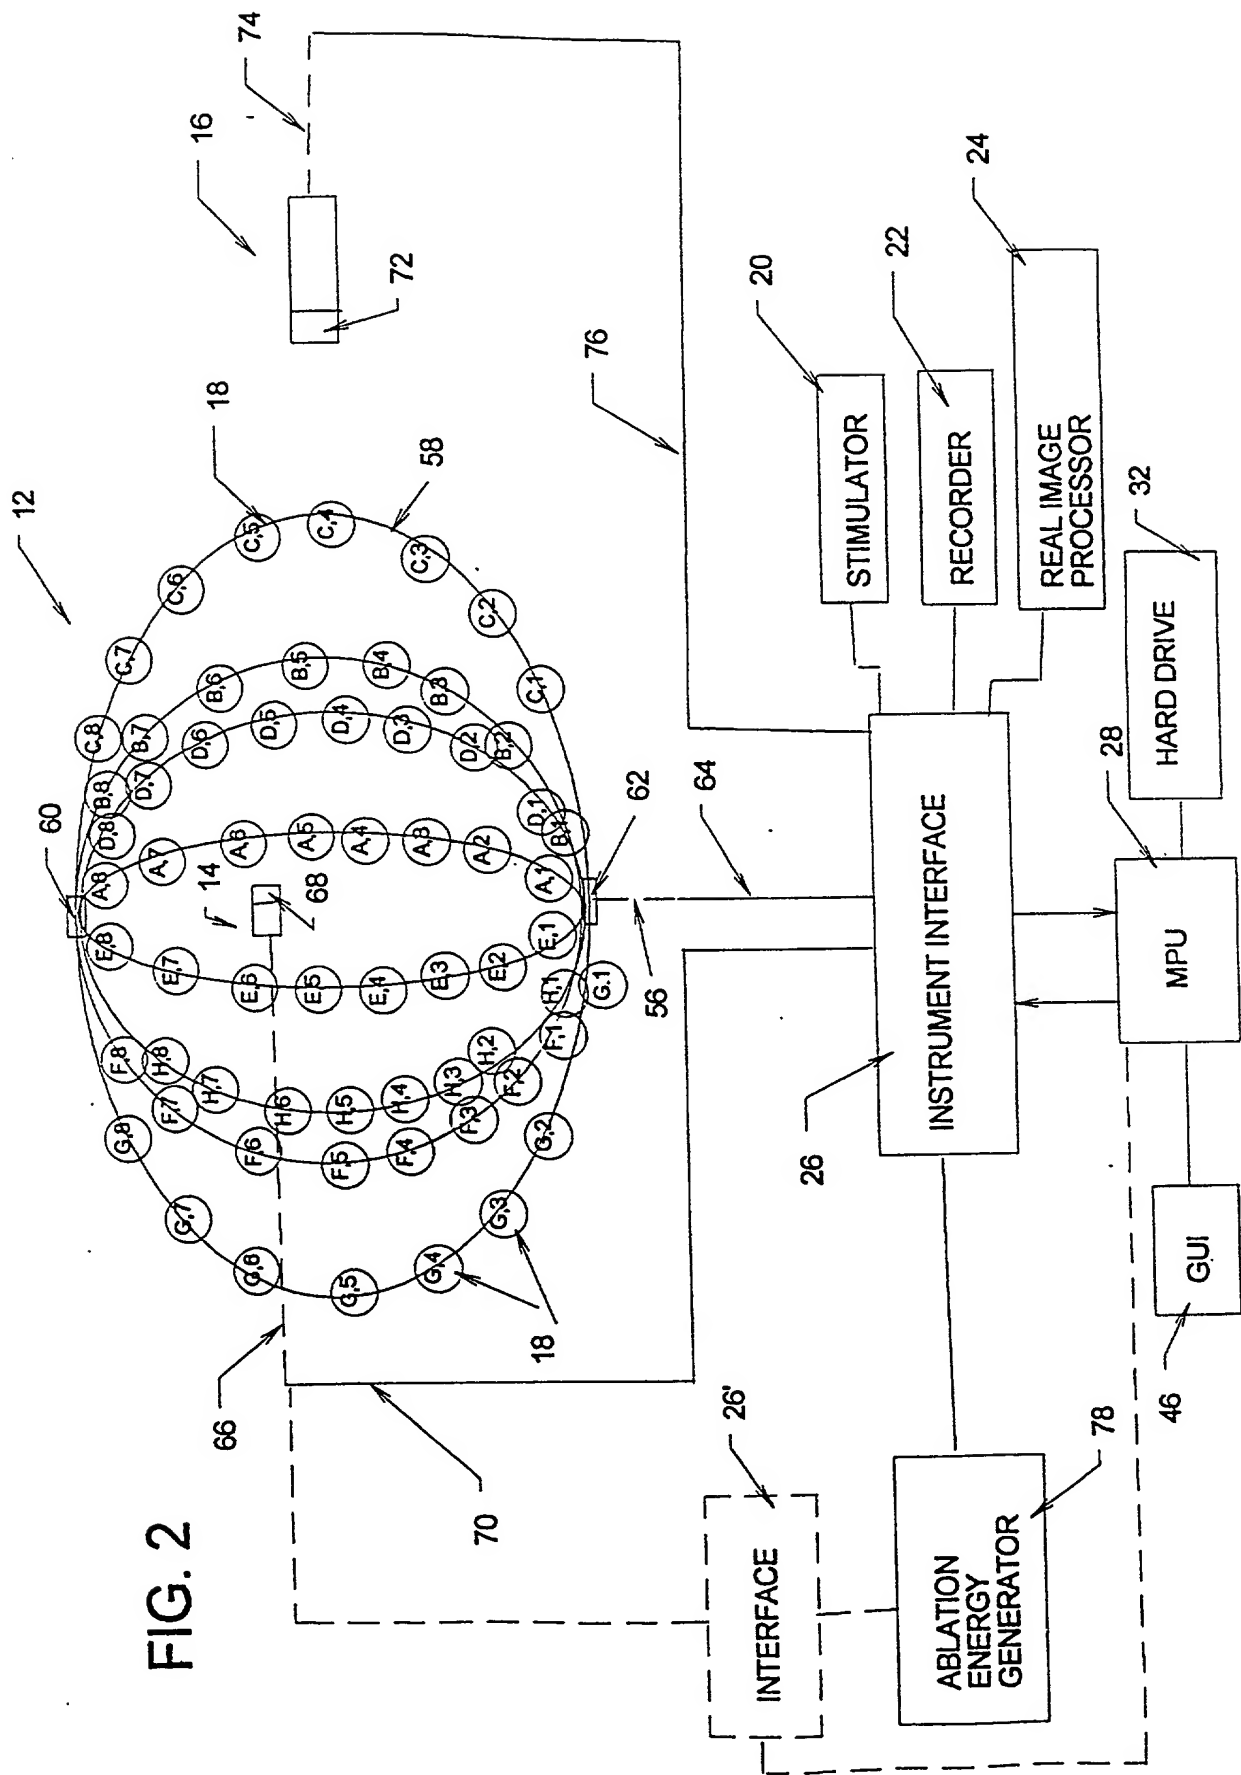


FIG. 1



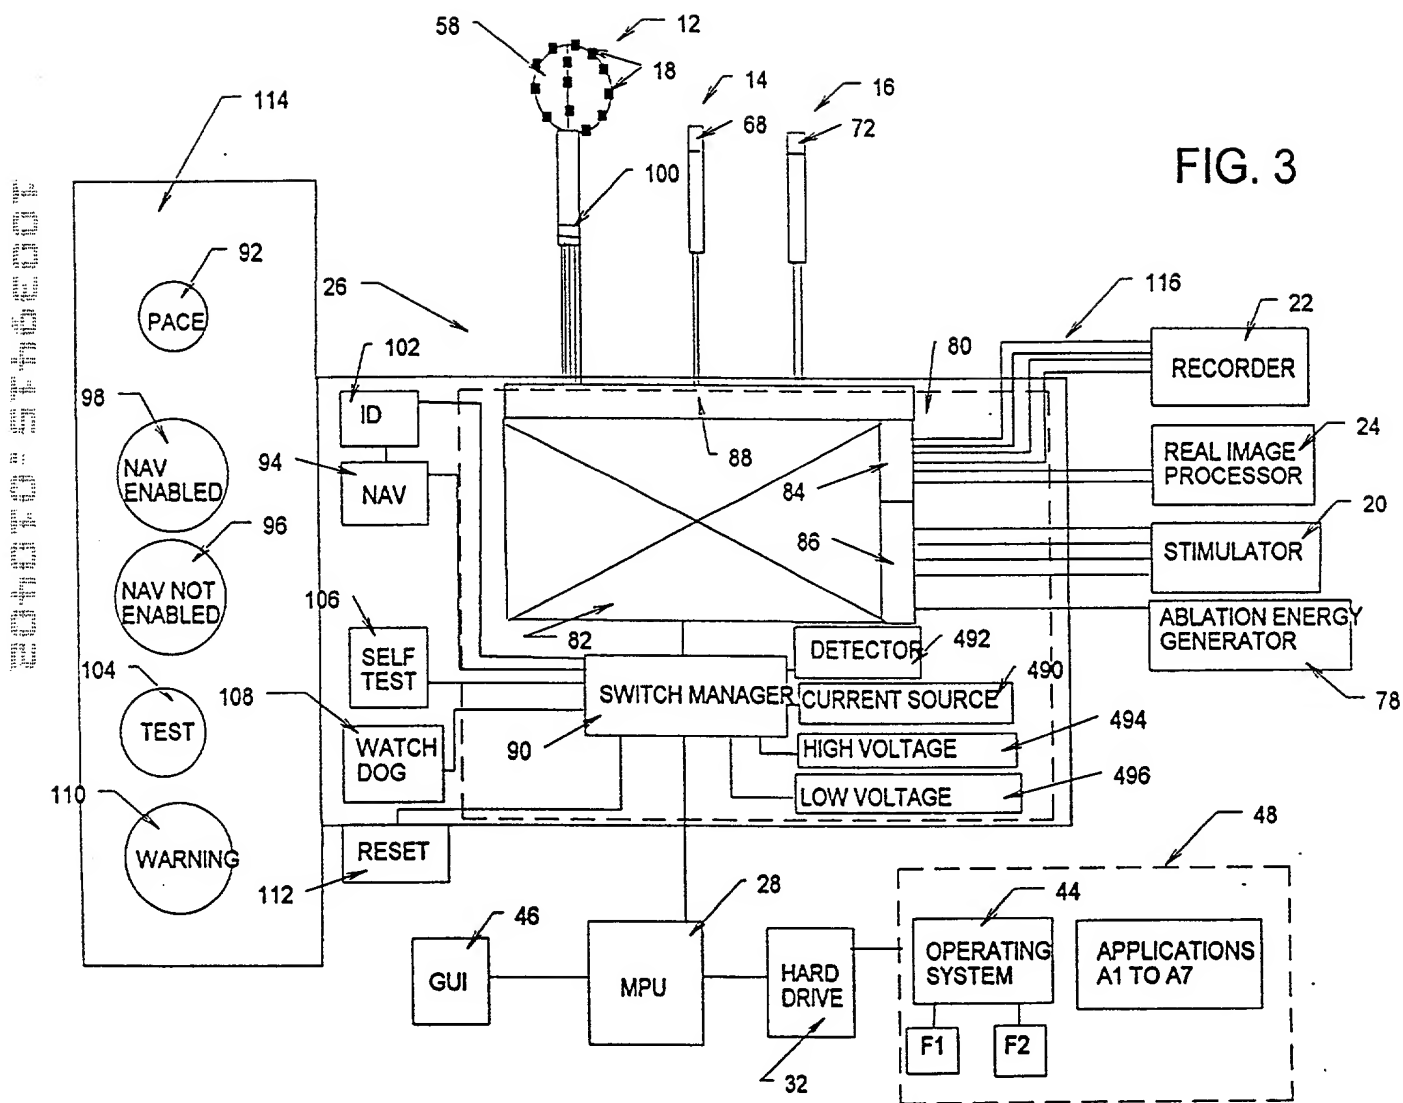


FIG. 4 is a schematic diagram of a start up screen of a medical device. The screen displays a logo and a menu of options. The options are: Recording Protocols, Pacing Protocols, Virtual Image Navigation, Real Image Navigation, Test, Print, Service, and Event Log OFF.

Start Up Screen
Logo

FIG. 4

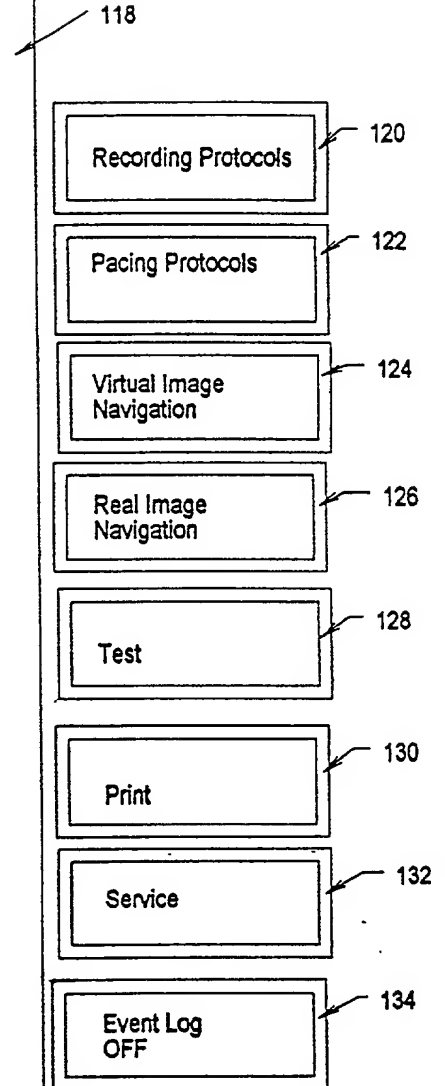


FIG. 5

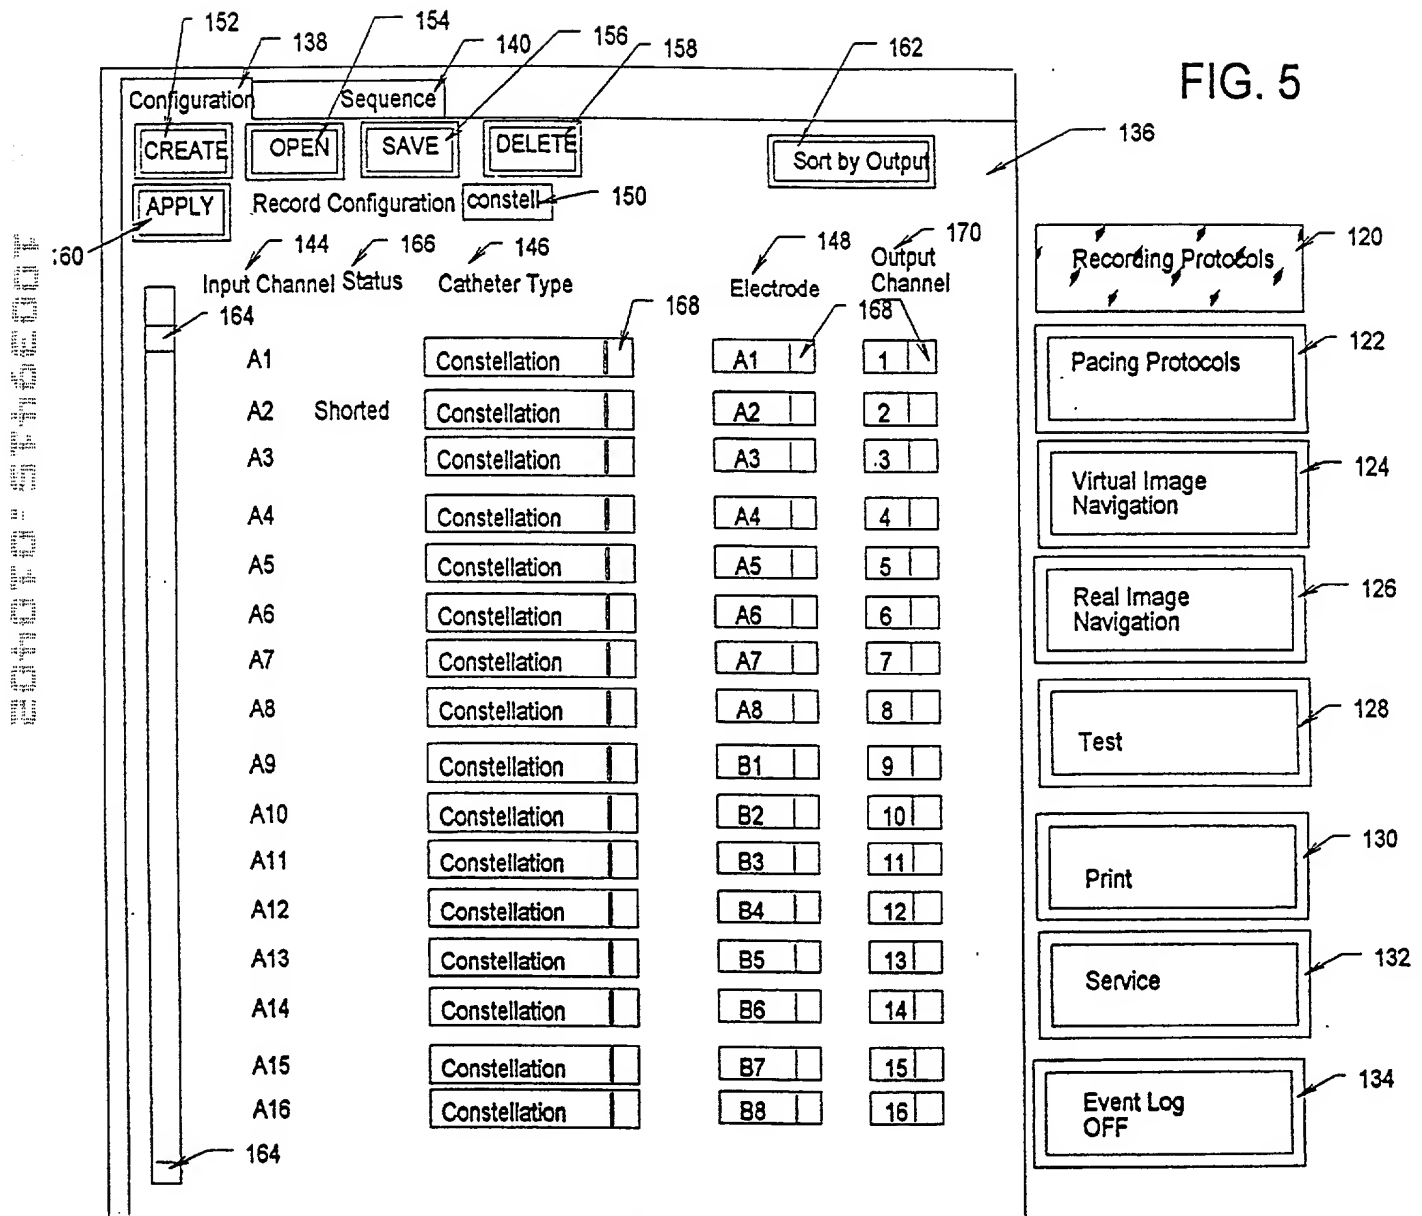


FIG. 6

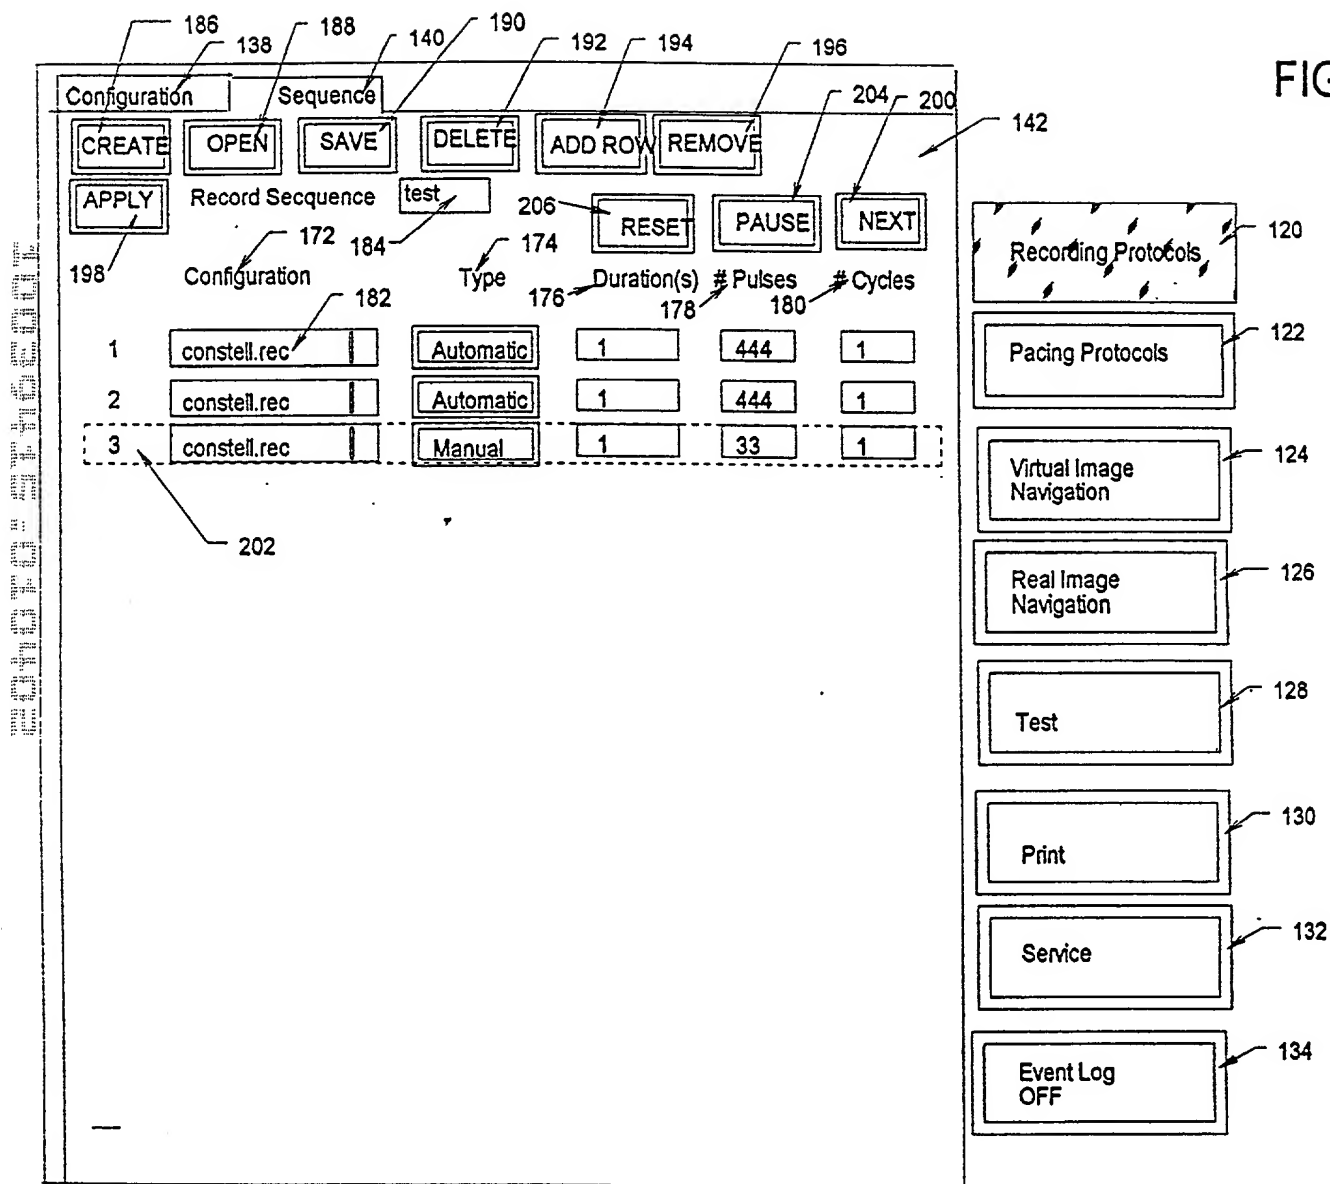


FIG. 7 is a block diagram of a user interface for a cardiac mapping system. The interface is divided into several functional areas. At the top, there are buttons for 'Configuration' (232), 'Sequence' (210), 'Pace Configuration' (234), and 'constell' (212). Below these are buttons for 'CREATE' (236), 'OPEN' (238), 'SAVE', and 'DELETE'. An 'APPLY' button is located below the 'CREATE' button. The main area of the interface is a table with columns for 'Input Channel Status' (216), 'Terminal Type' (226), 'Electrode' (220), and 'Terminal' (222). The table lists 16 input channels (A1 through A16). Channels A1 through A14 are marked as 'Constellation' under 'Terminal Type'. Channels A15 and A16 are marked as 'Constellation' under 'Terminal Type'. The 'Electrode' column lists A1 through A8, B1 through B8. The 'Terminal' column lists 1-, 1+, None, 2+, 2-, None. To the right of the table, there are several buttons: 'Disconnect stim. Inputs' (242), 'Recording Protocols' (120), 'Pacing Protocols' (122), 'Virtual Image Navigation' (124), 'Real Image Navigation' (126), 'Test' (128), 'Print' (130), 'Service' (132), and 'Event Log OFF' (134). The interface is labeled 'FIG. 7'.

Configuration

Sequence

Pace Configuration

constell

CREATE

OPEN

SAVE

DELETE

APPLY

Input Channel	Status	Terminal Type	Electrode	Terminal
A1		Constellation	A1	1-
A2	Shorted	Constellation	A2	1+
A3		Constellation	A3	None
A4		Constellation	A4	2+
A5		Constellation	A5	2-
A6		Constellation	A6	None
A7		Constellation	A7	None
A8		Constellation	A8	None
A9		Constellation	B1	None
A10		Constellation	B2	None
A11		Constellation	B3	None
A12		Constellation	B4	None
A13		Constellation	B5	None
A14		Constellation	B6	None
A15		Constellation	B7	None
A16		Constellation	B8	None

Disconnect stim. Inputs

Recording Protocols

Pacing Protocols

Virtual Image Navigation

Real Image Navigation

Test

Print

Service

Event Log OFF

FIG. 7

FIG. 8

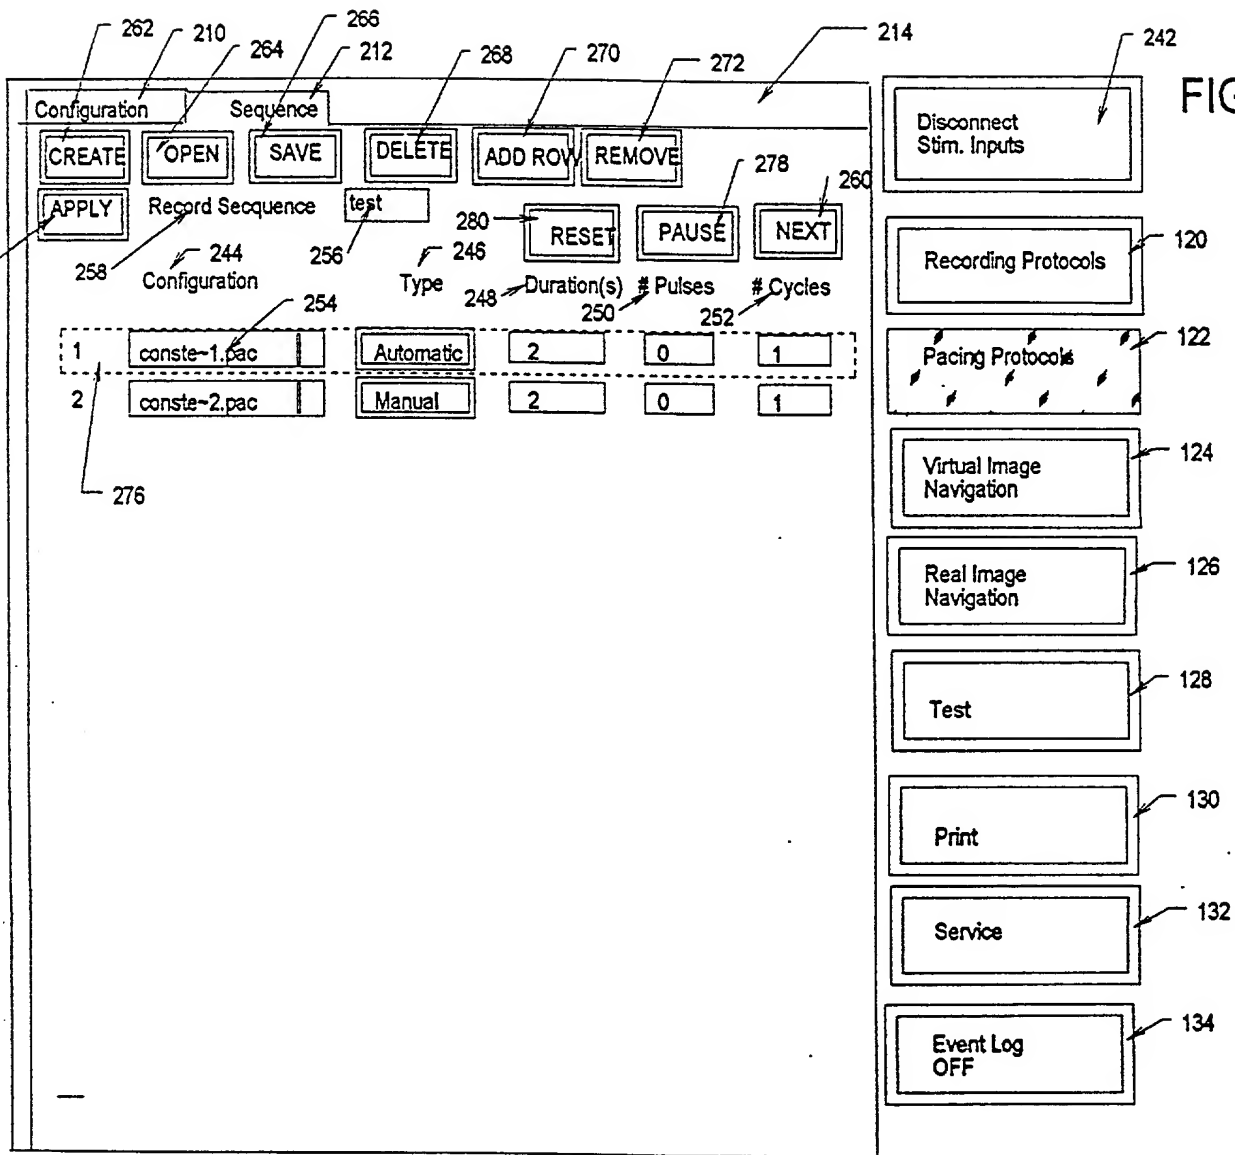


FIG. 8

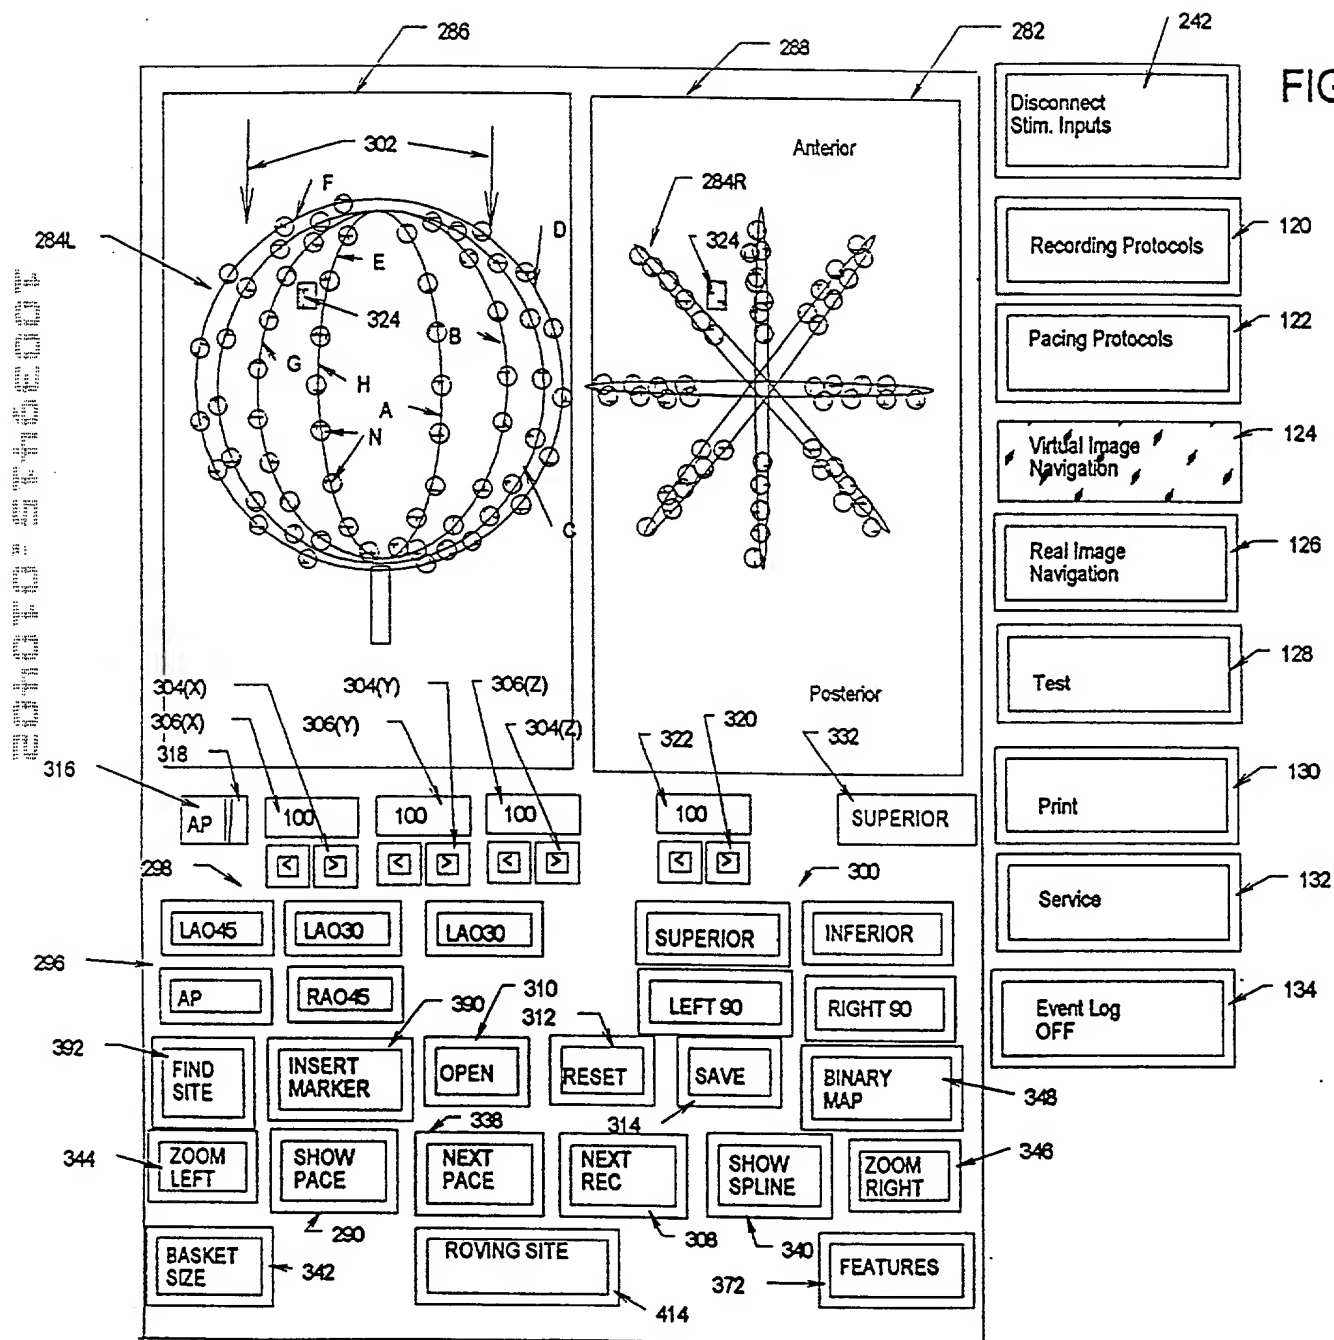


FIG. 10

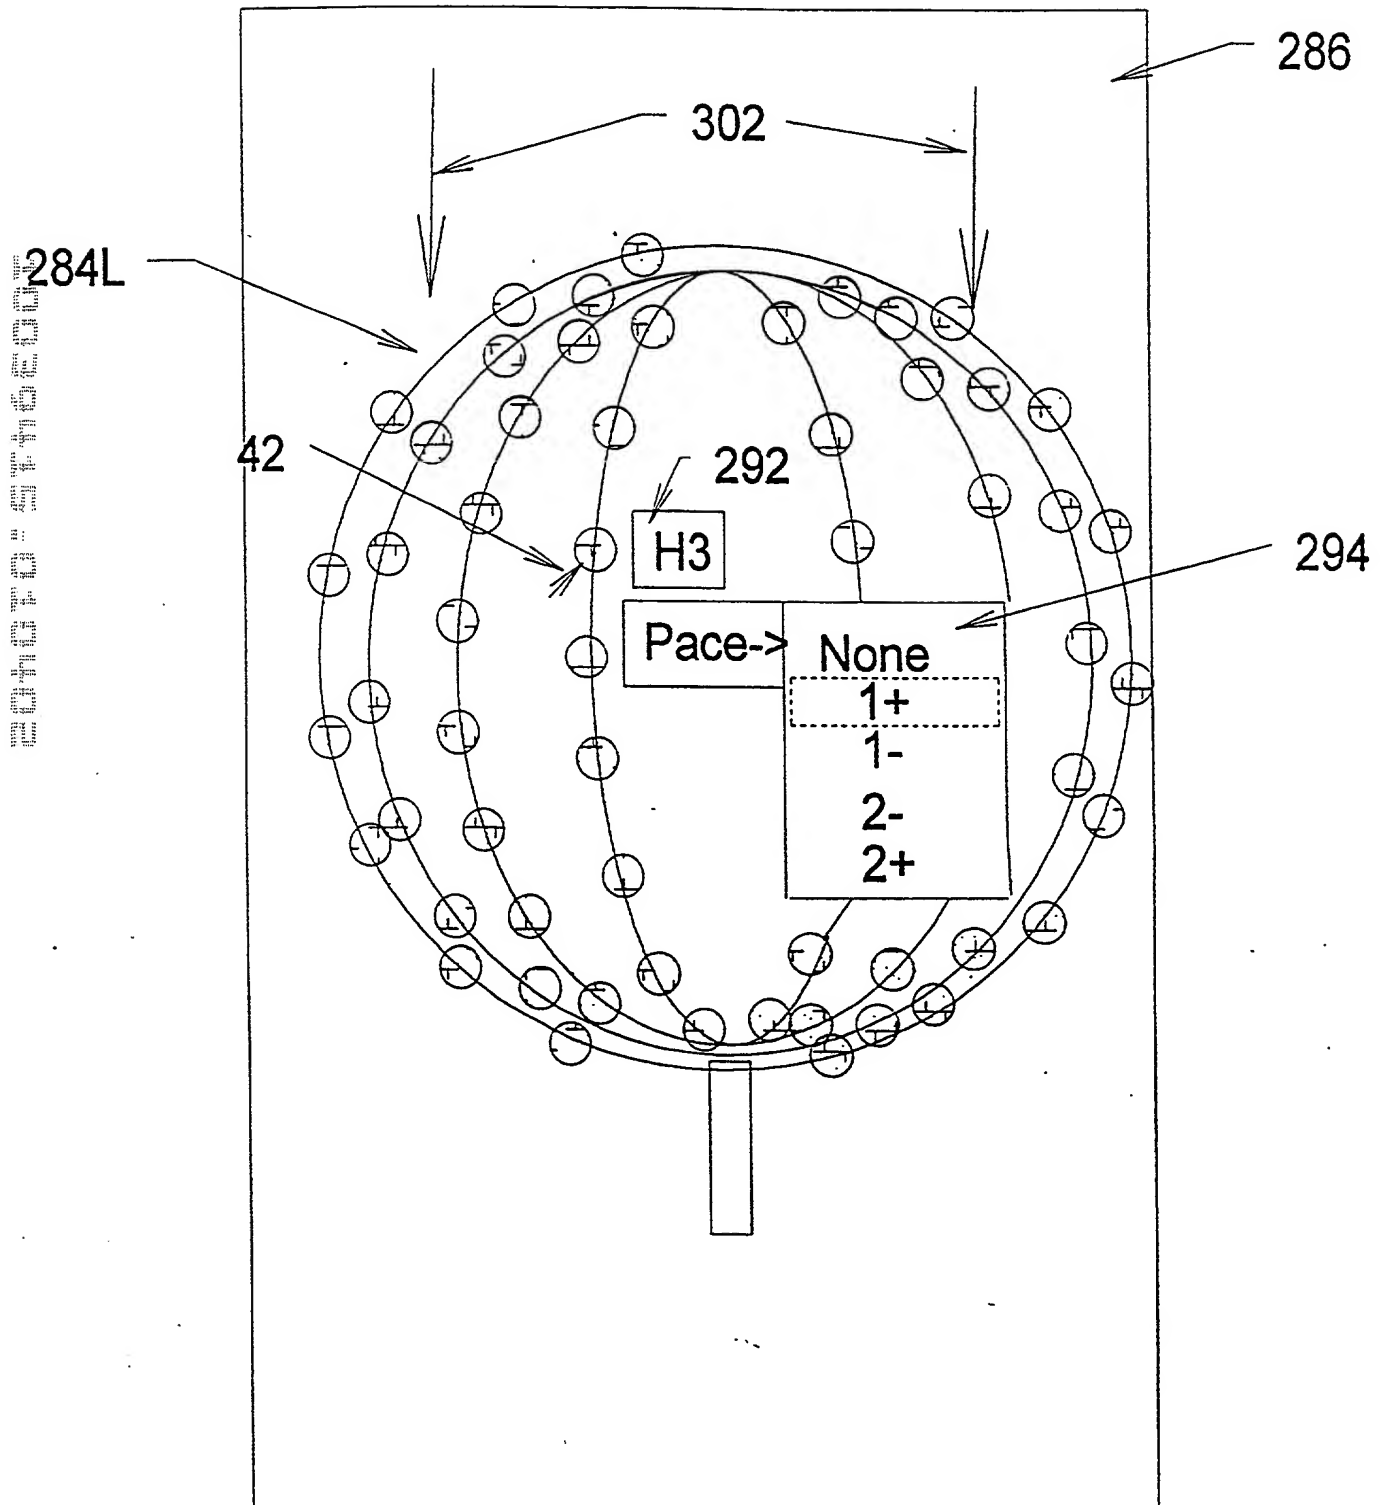


FIG. 11

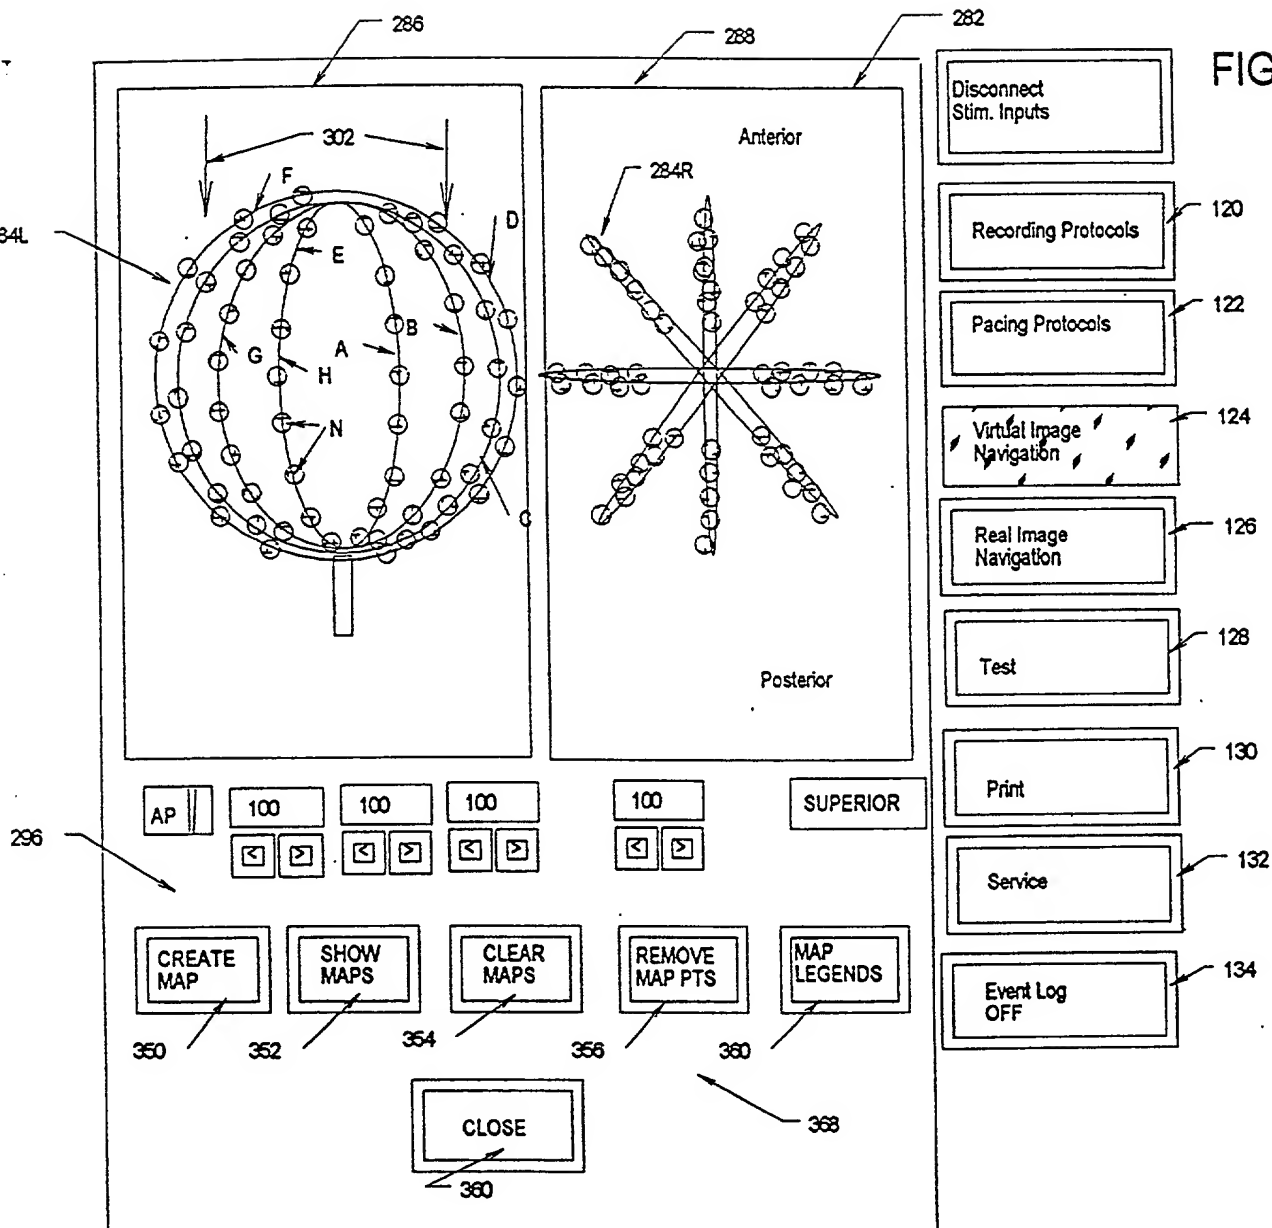


FIG. 11

FIG. 12

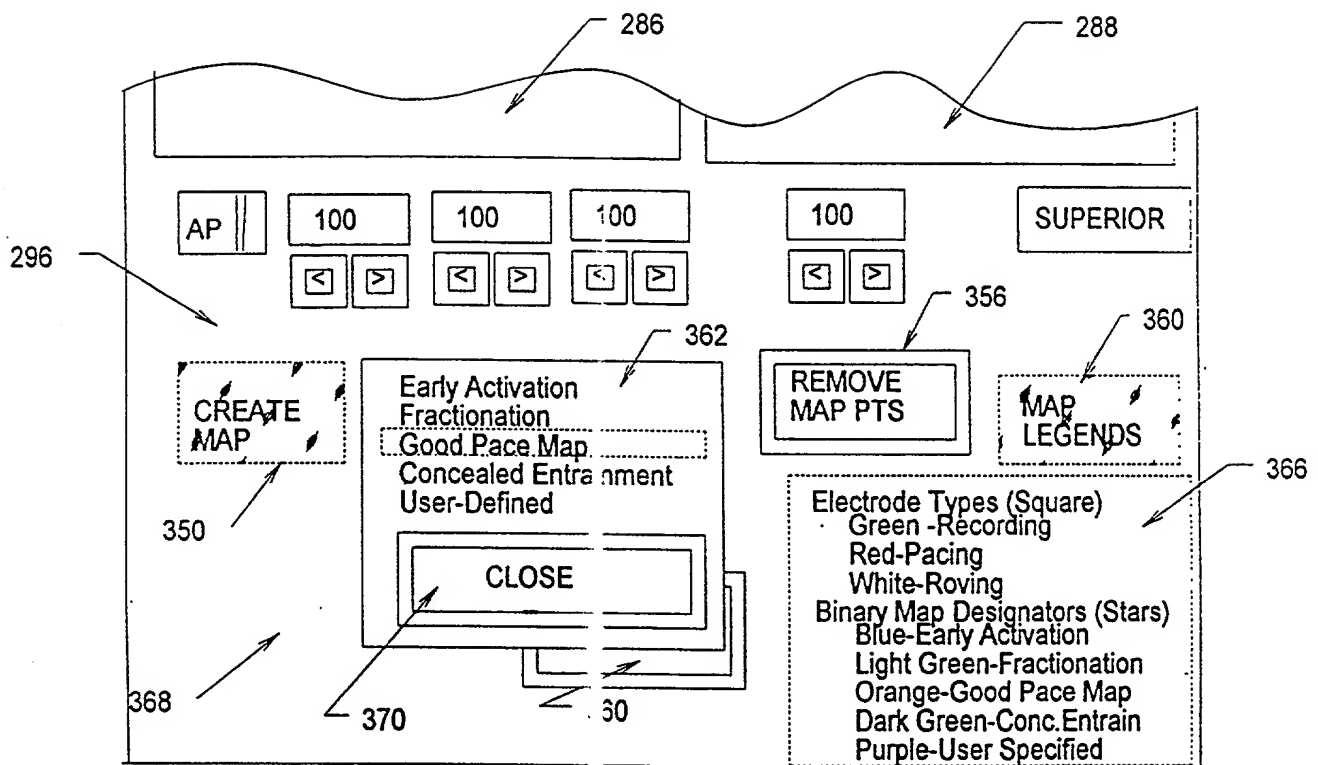
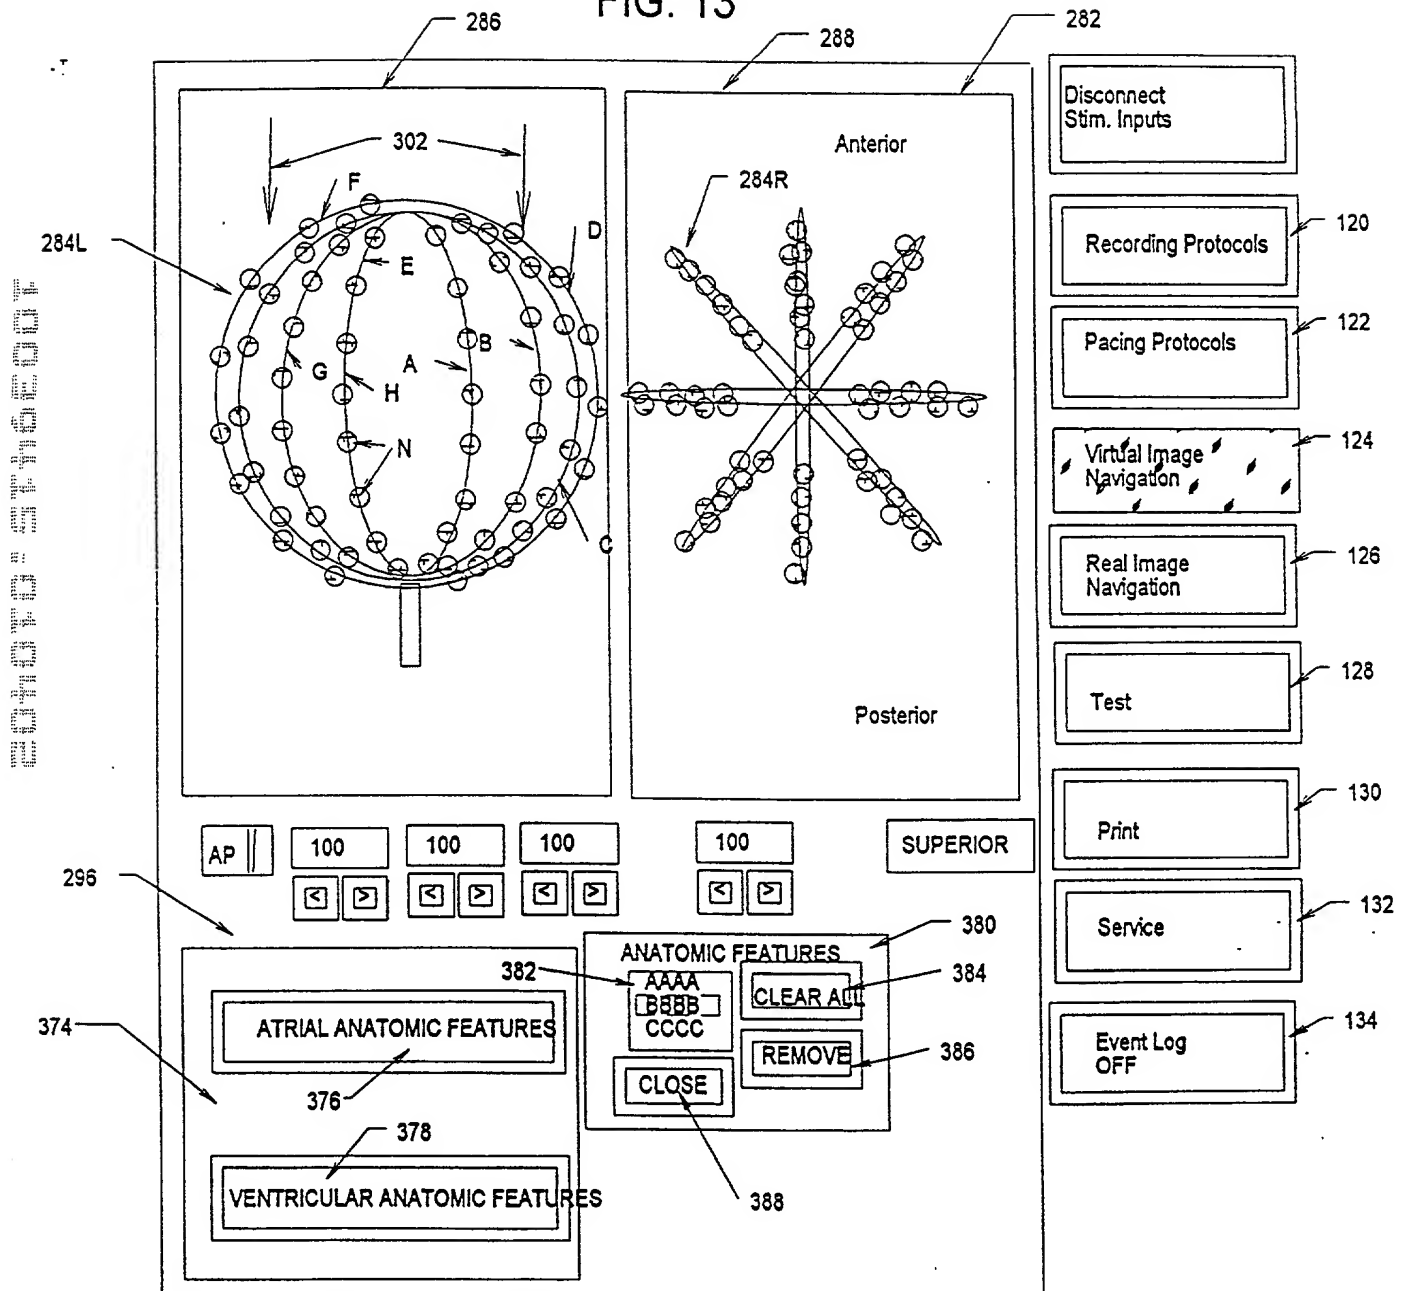


FIG. 13



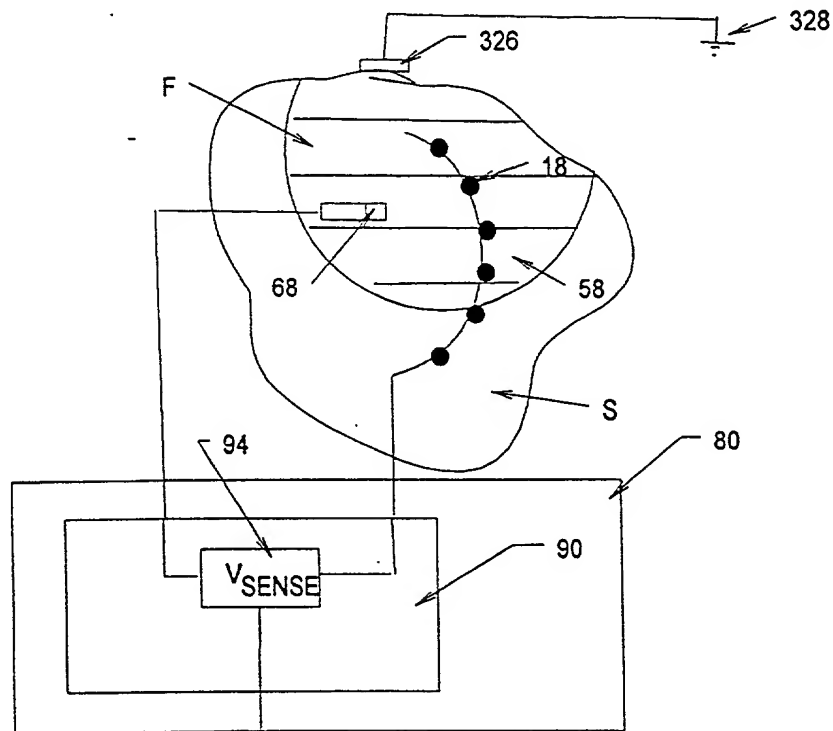


FIG. 14

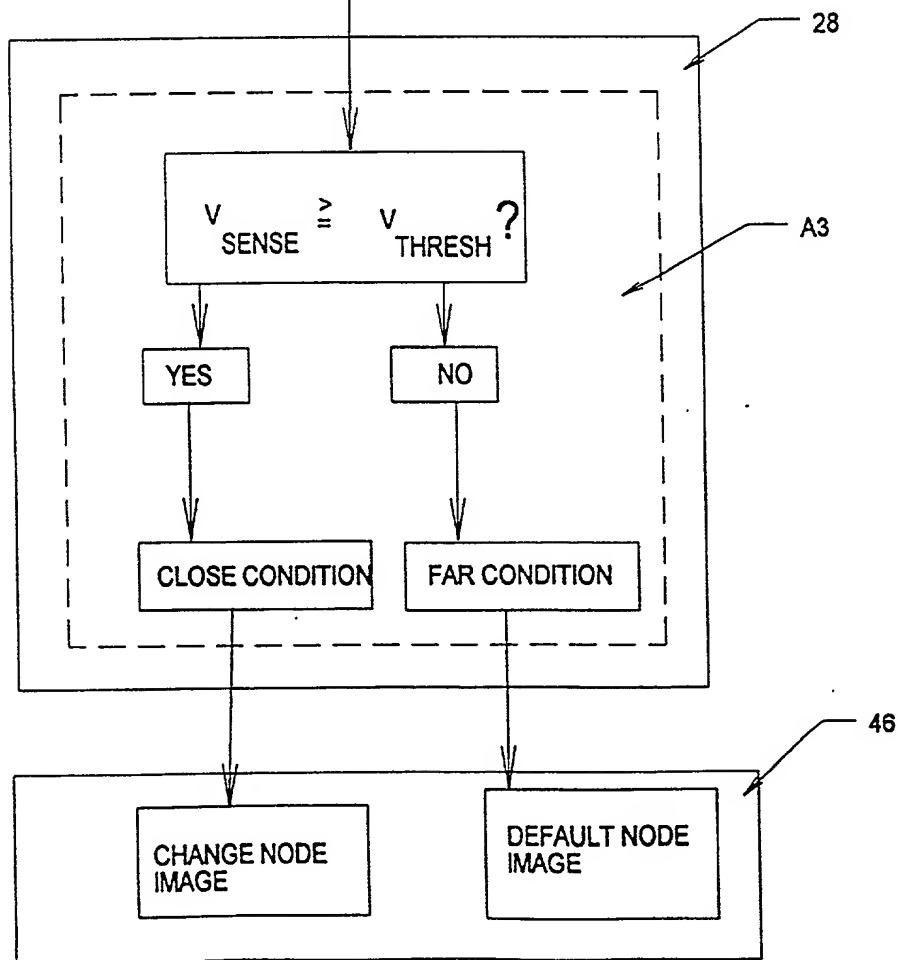


FIG. 15

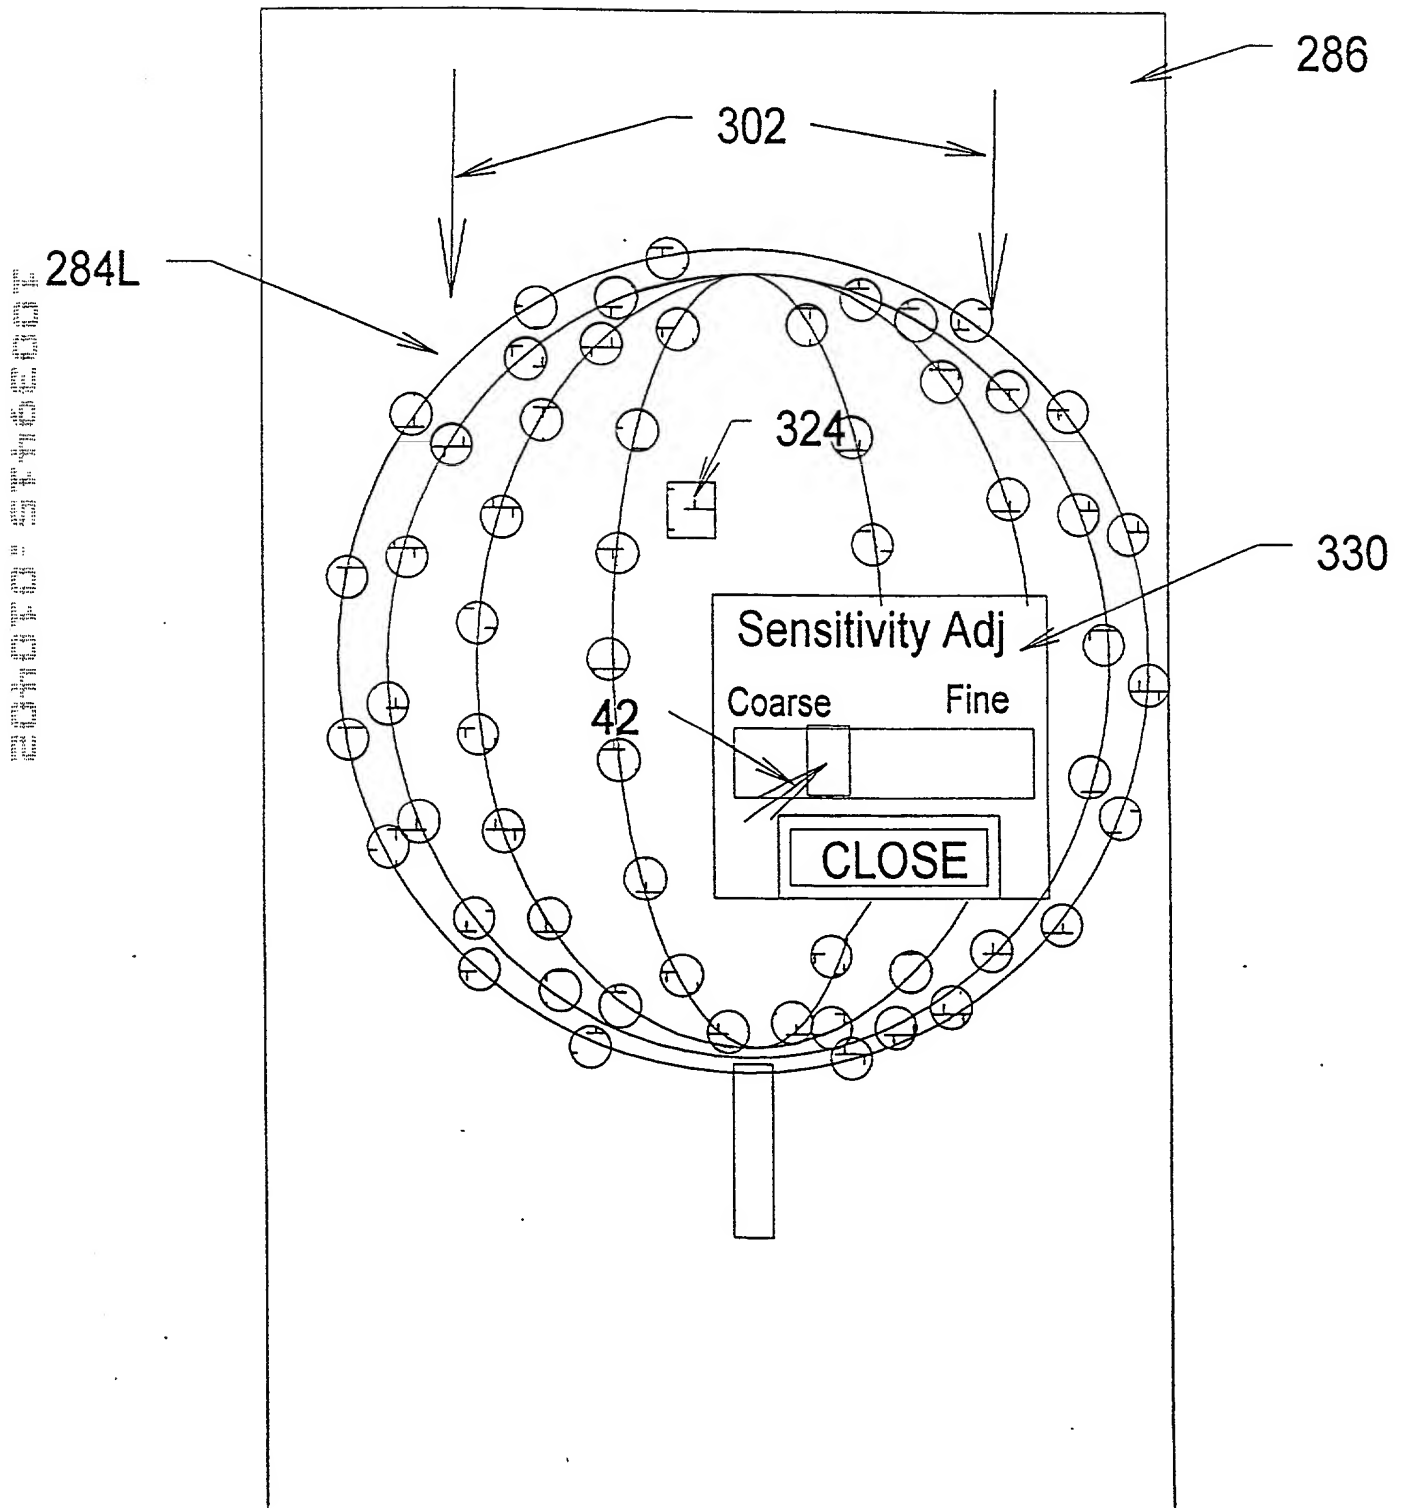


FIG. 16

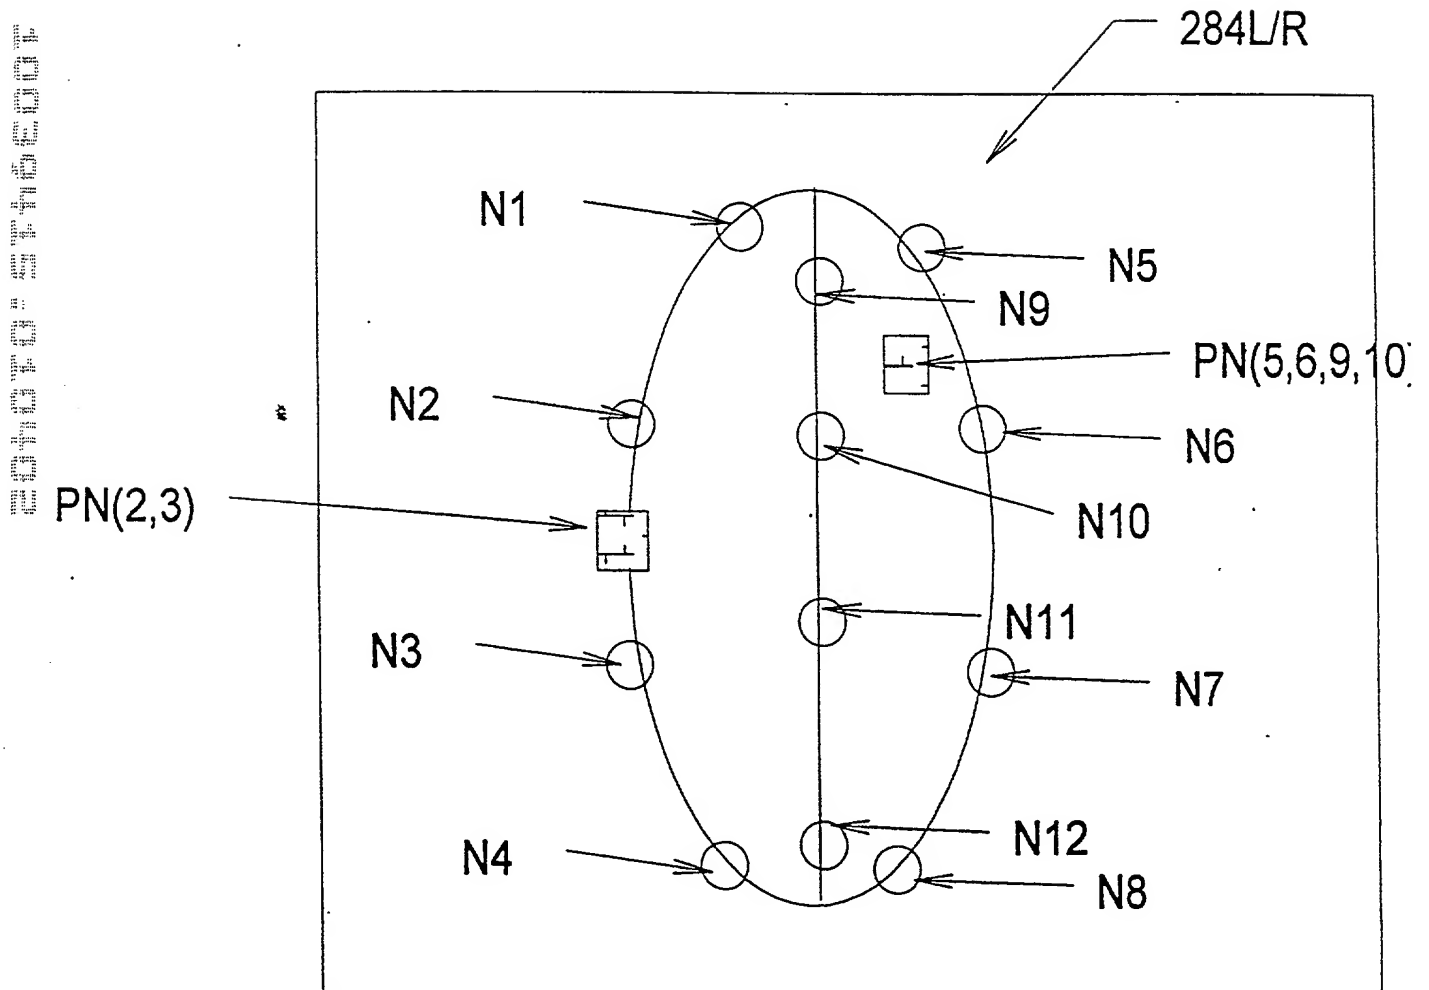


FIG. 17

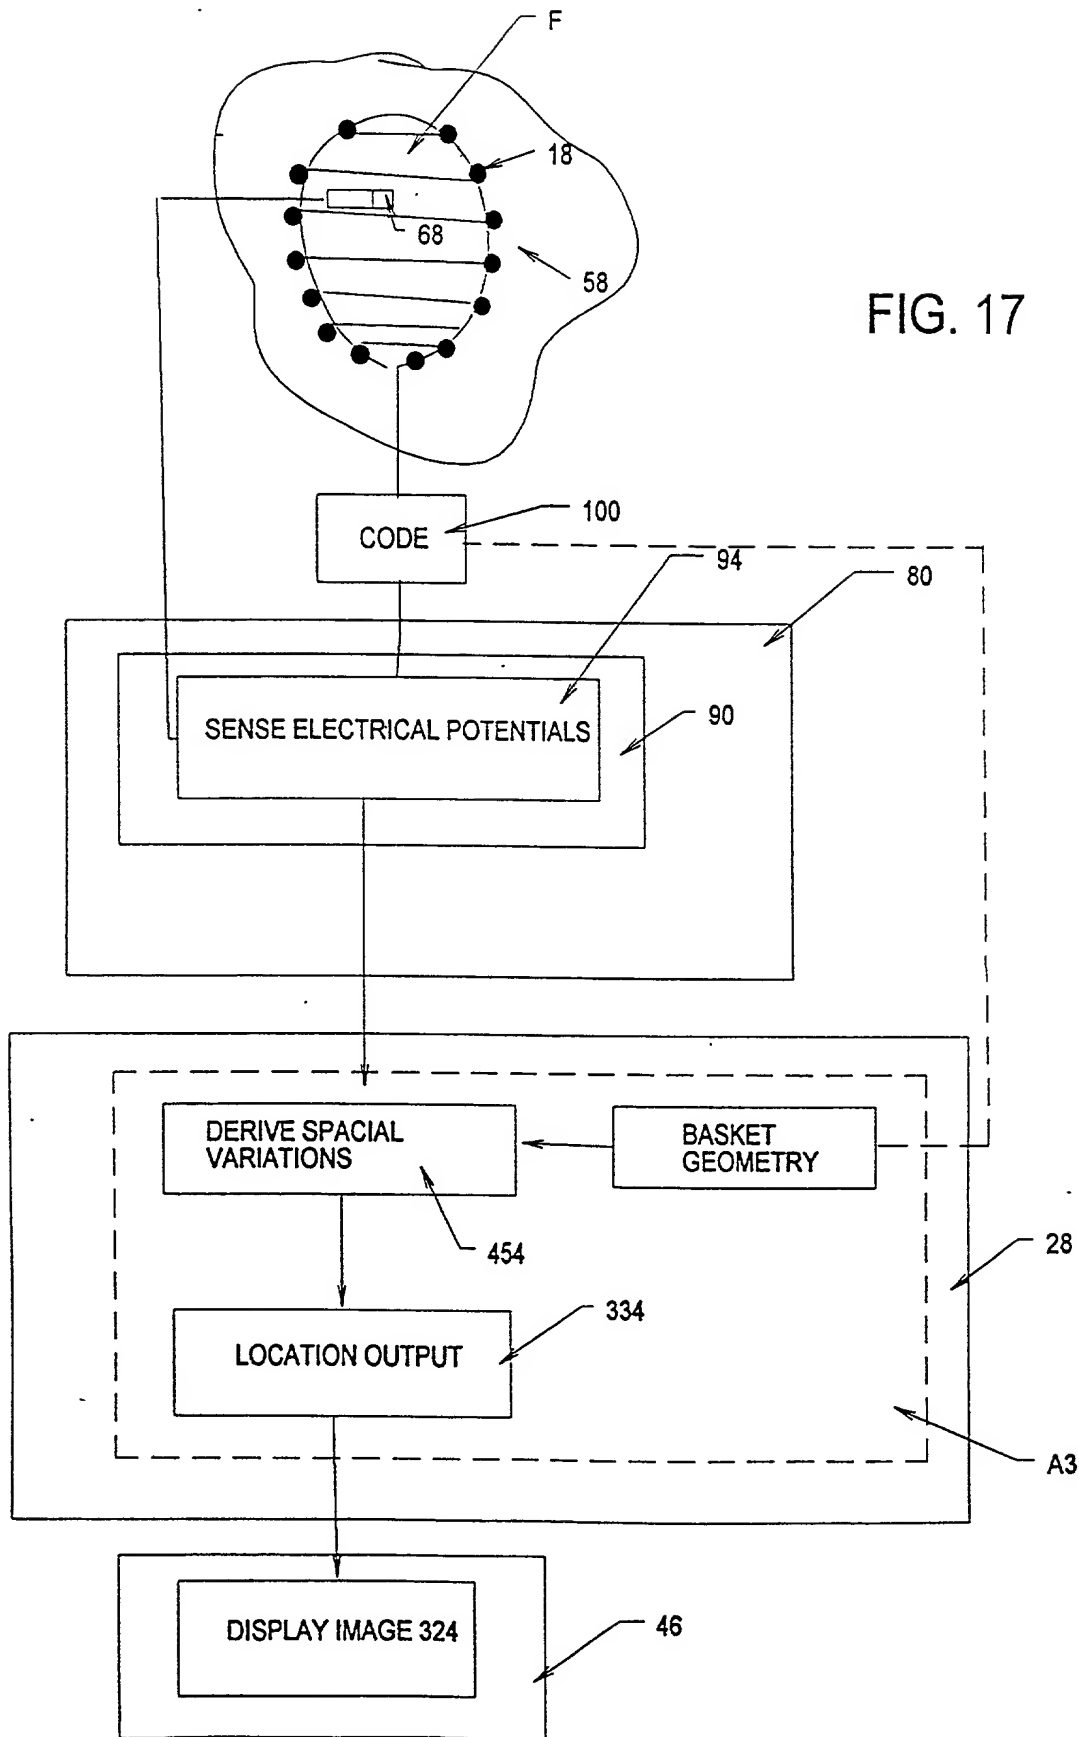


FIG. 18

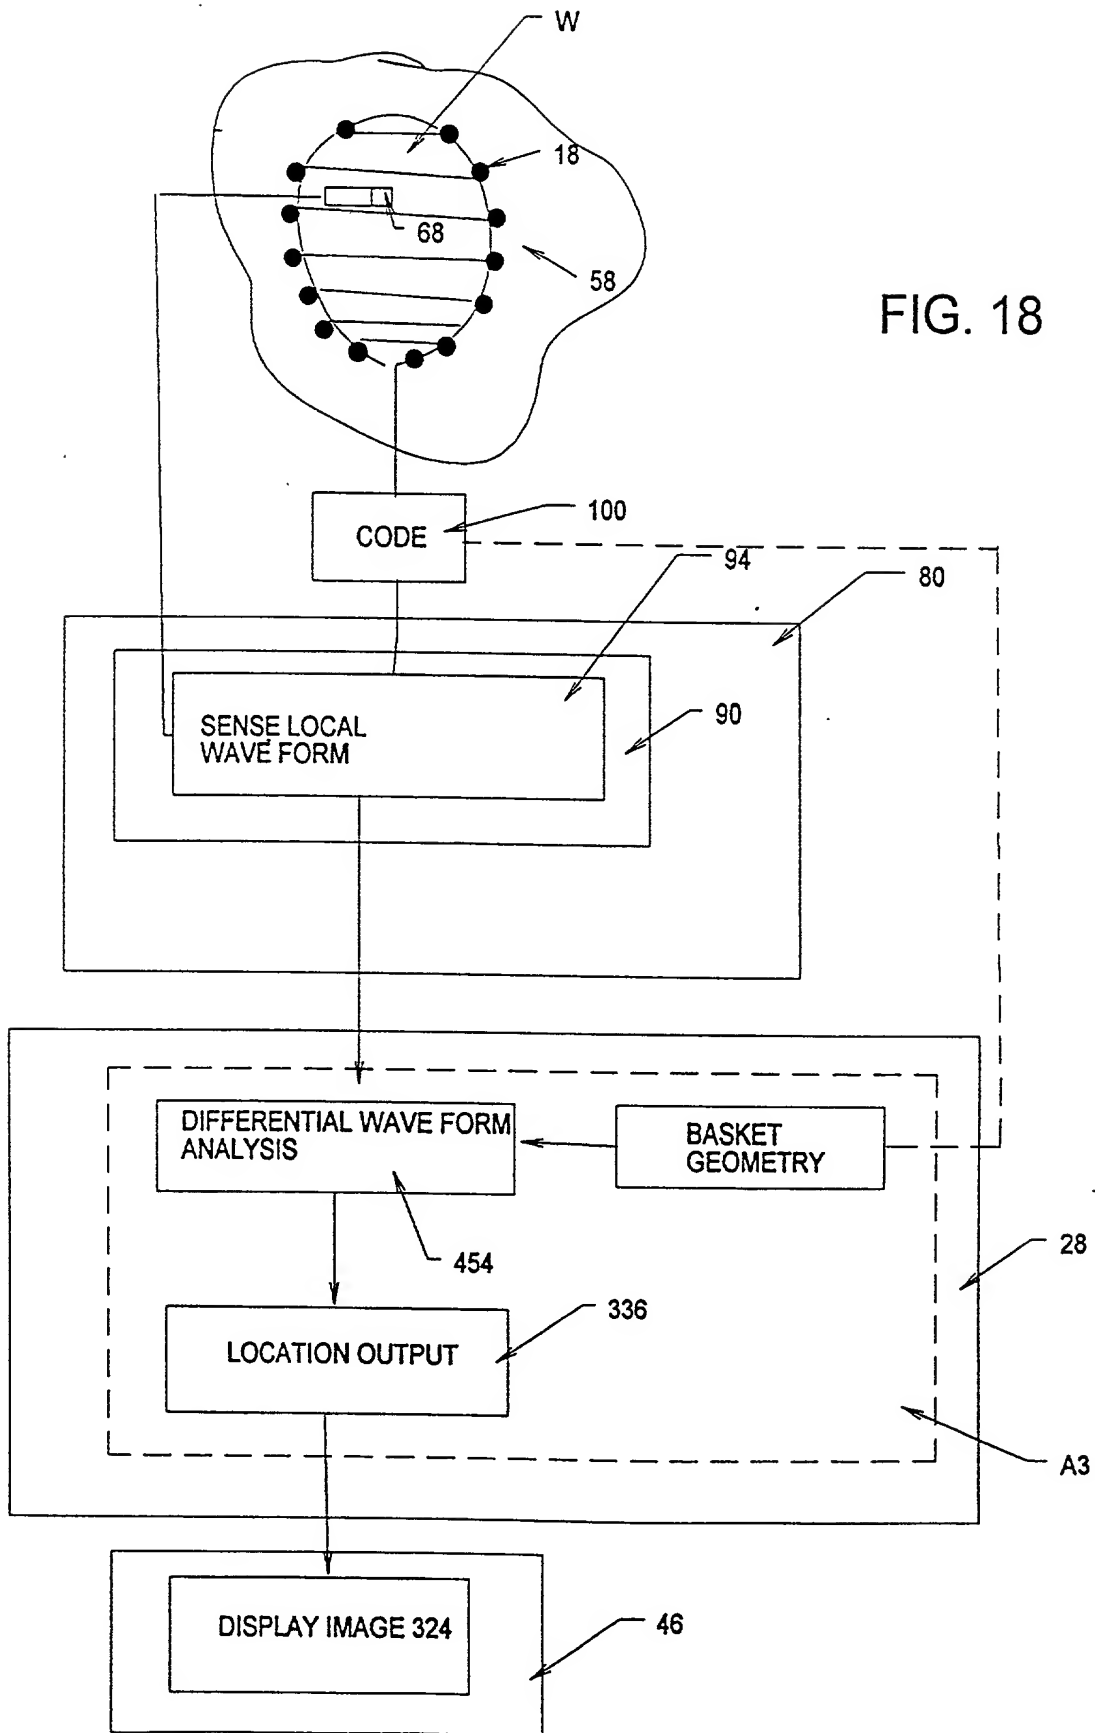


FIG. 19

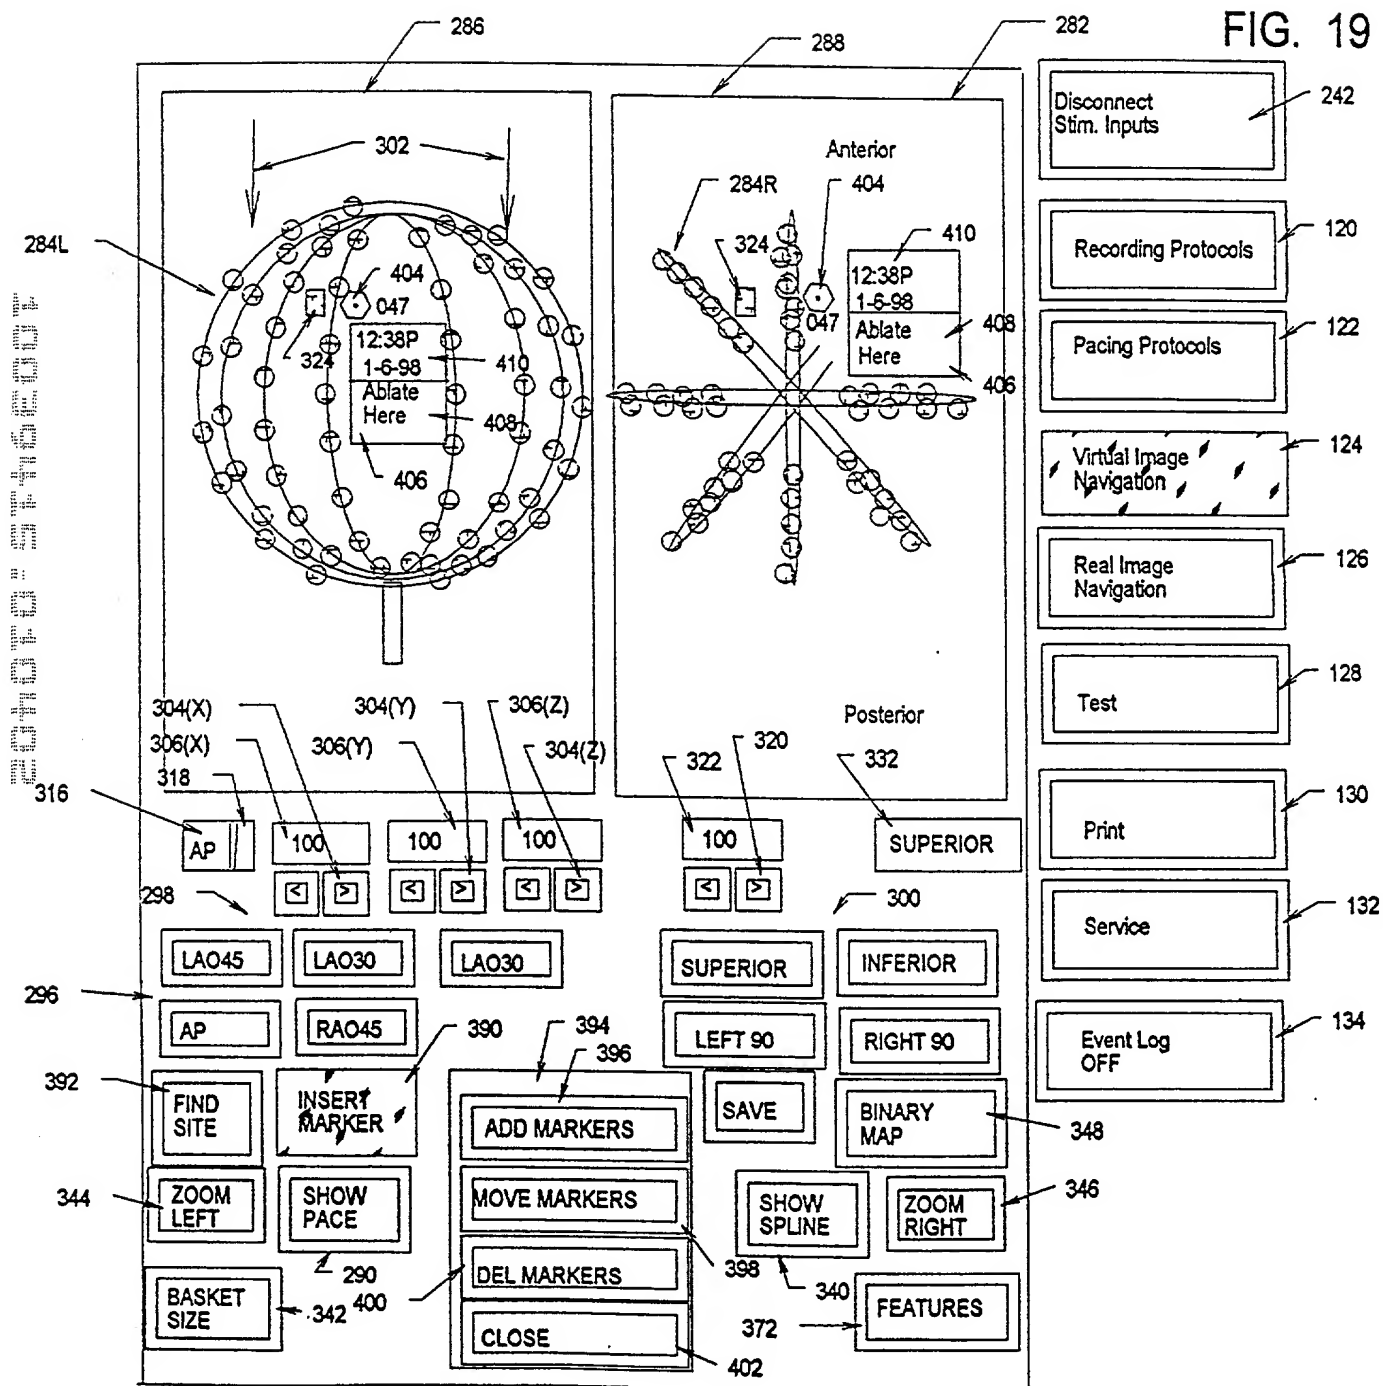


FIG. 20

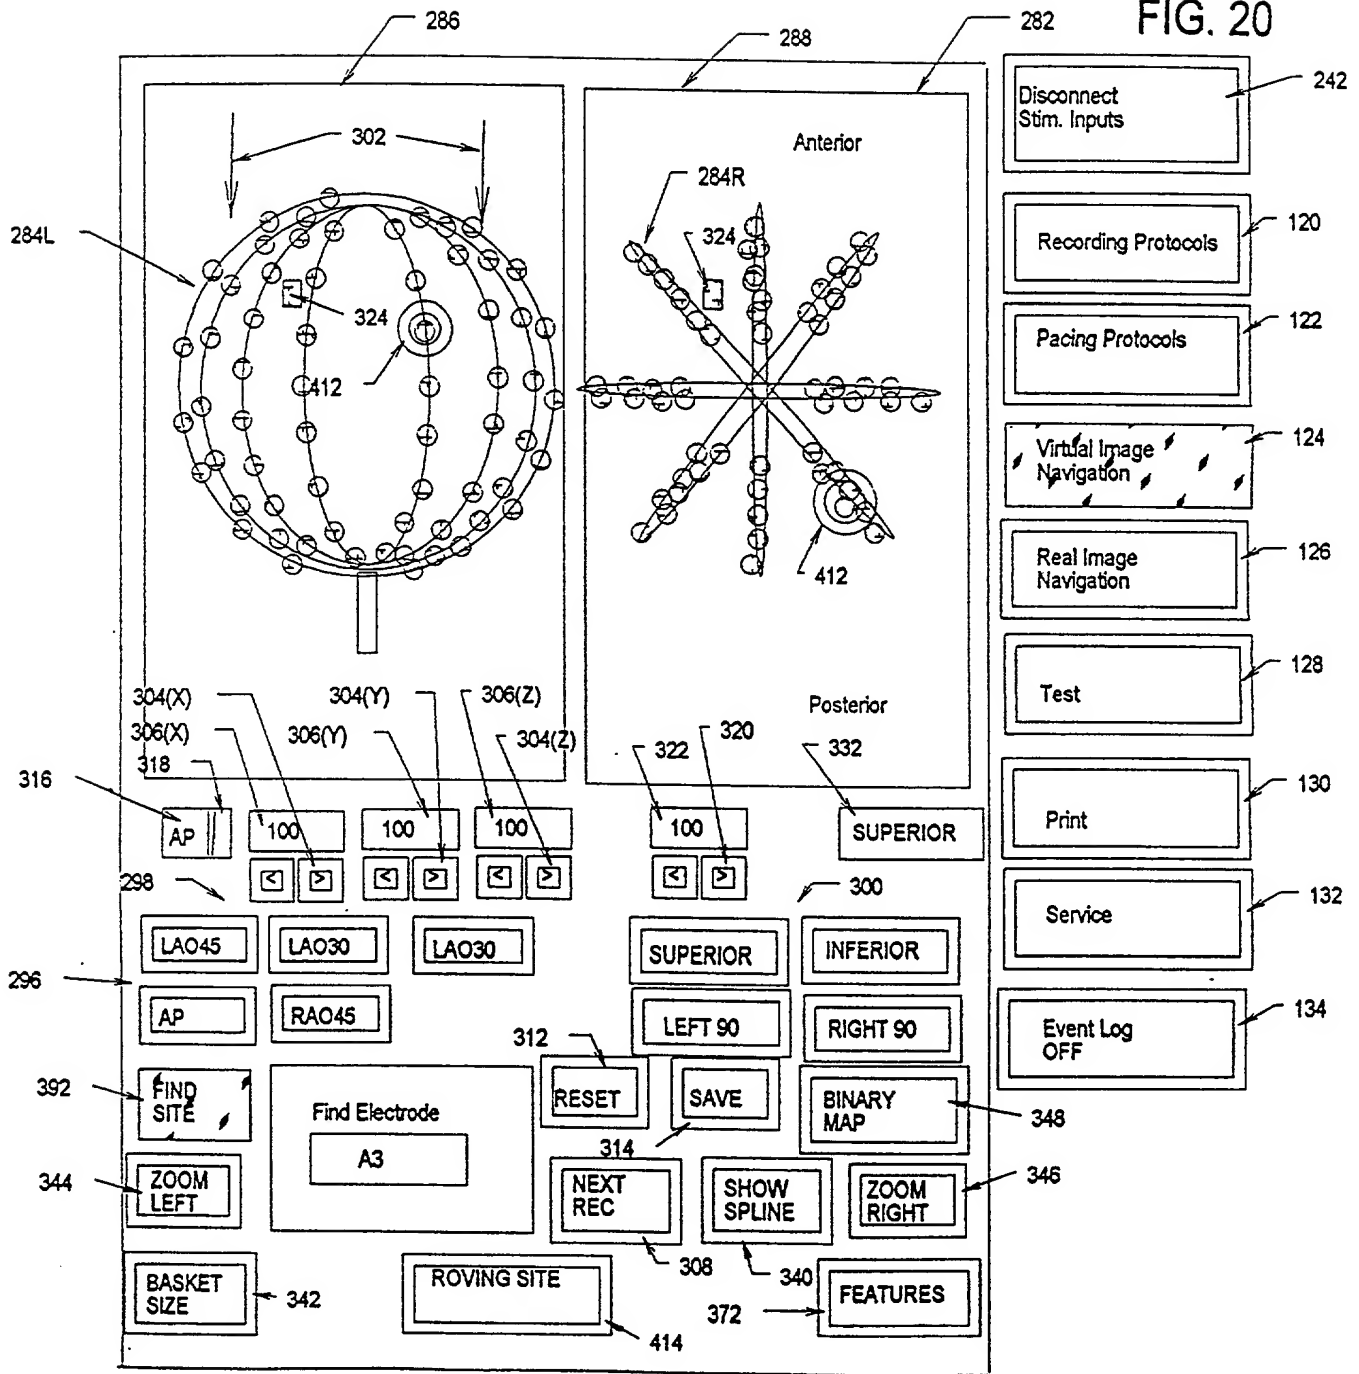


FIG. 21

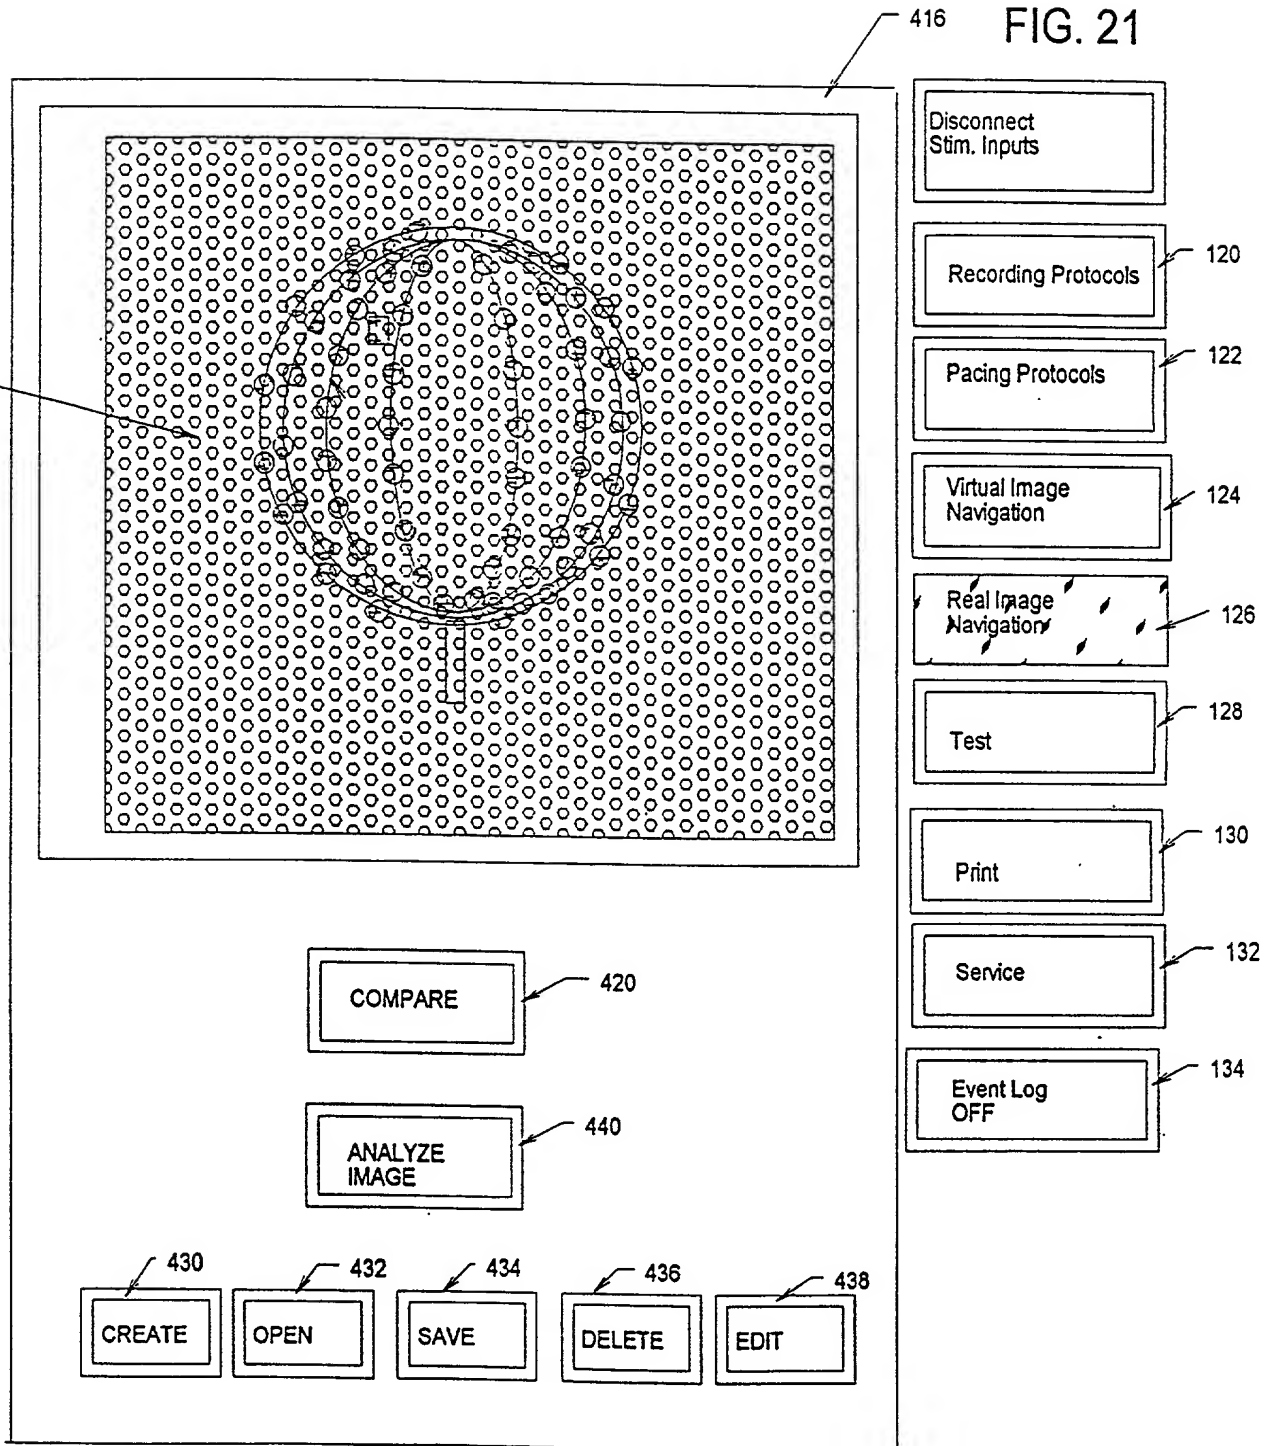
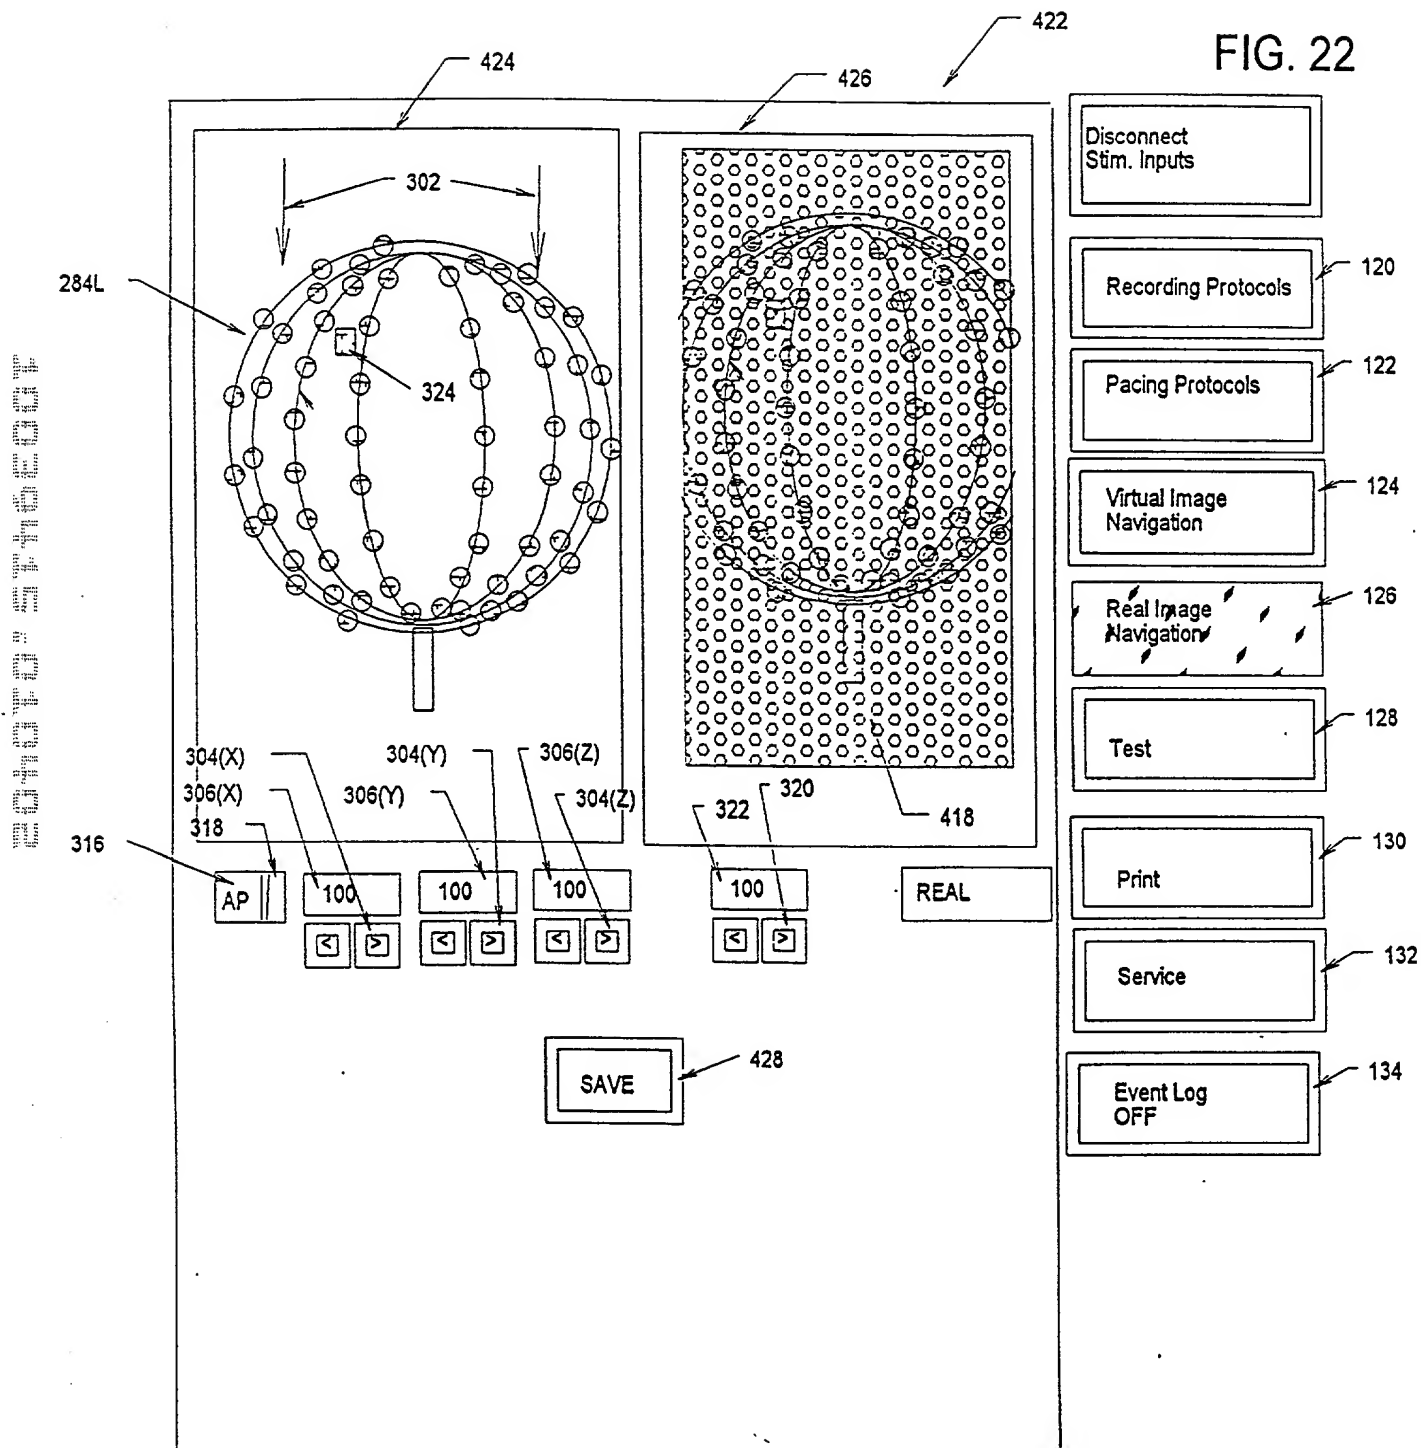


FIG. 22



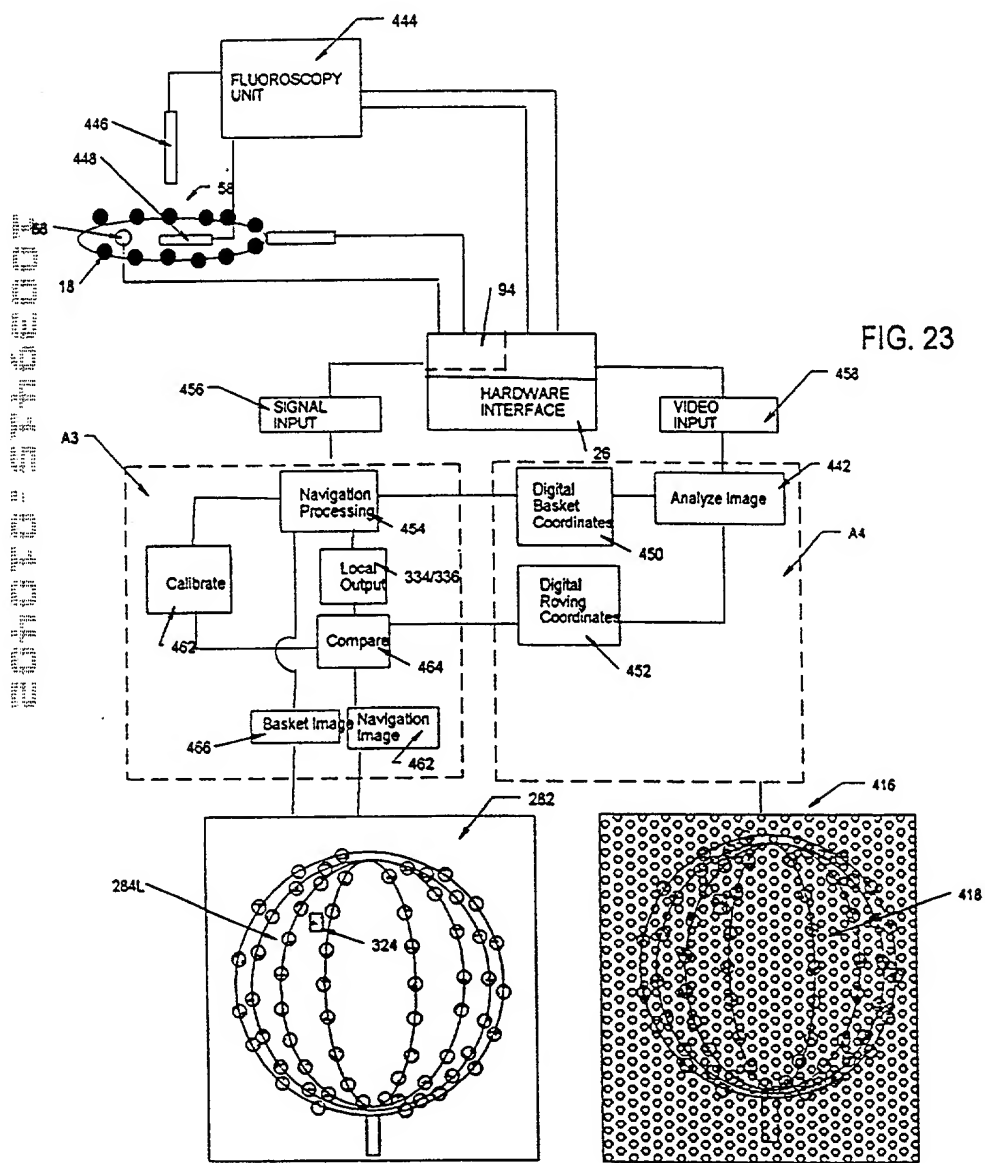


FIG. 24

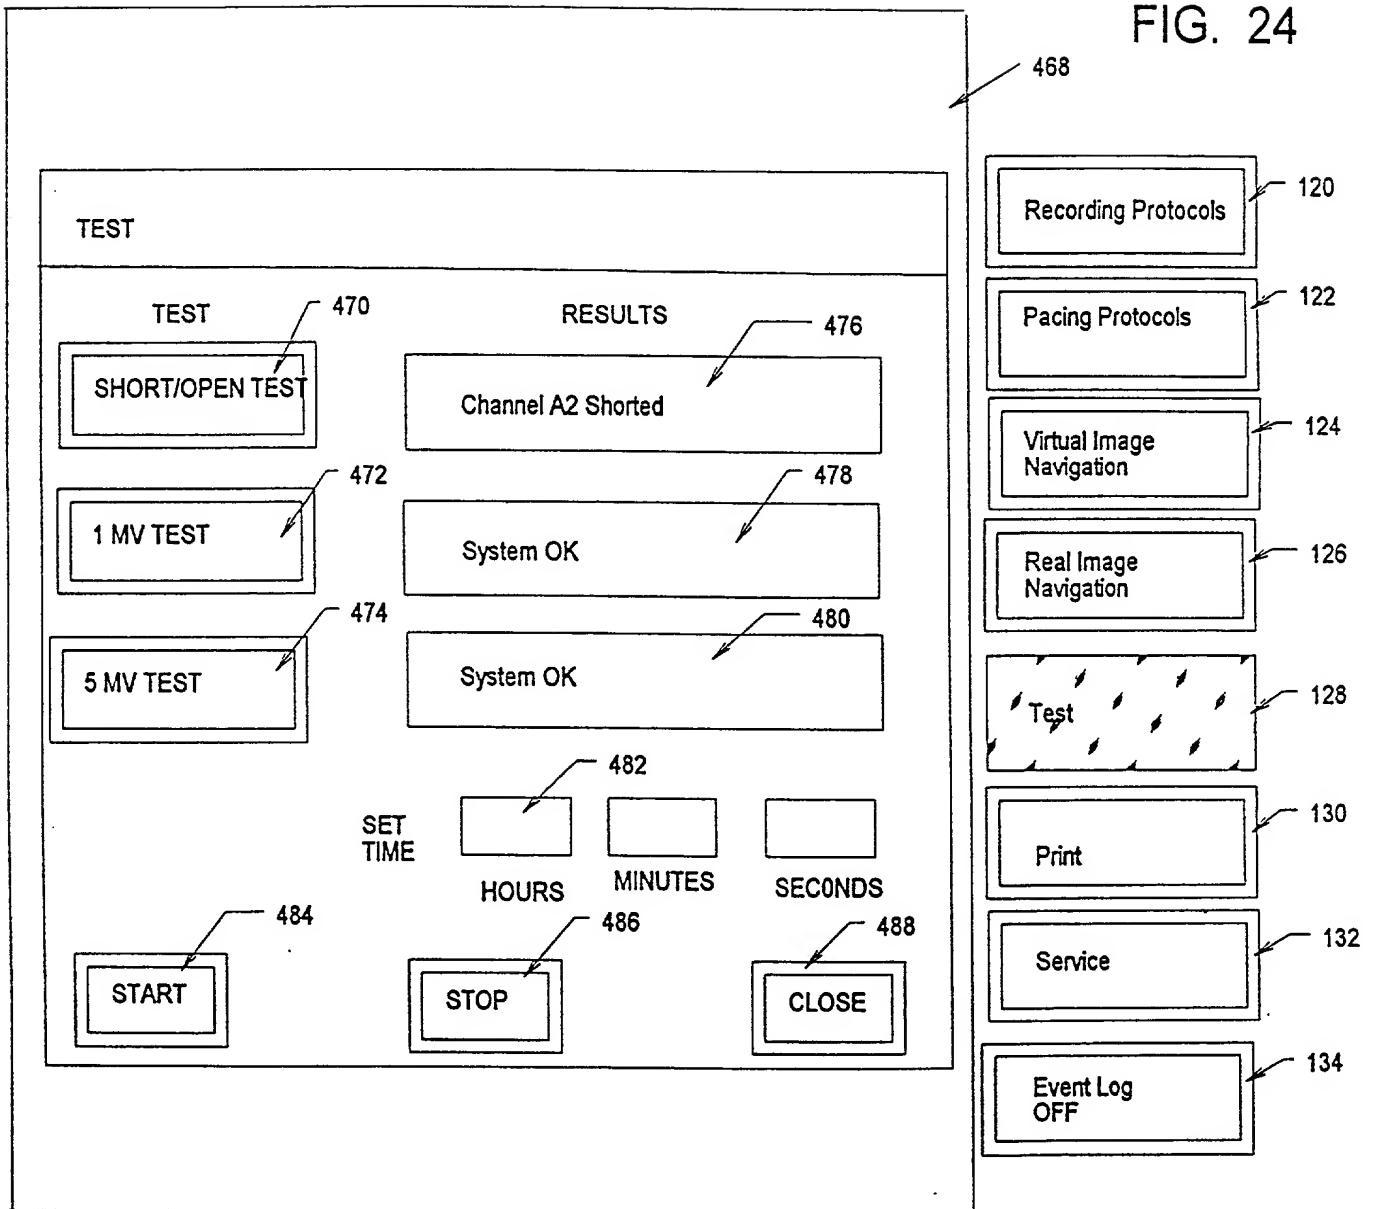


FIG. 25

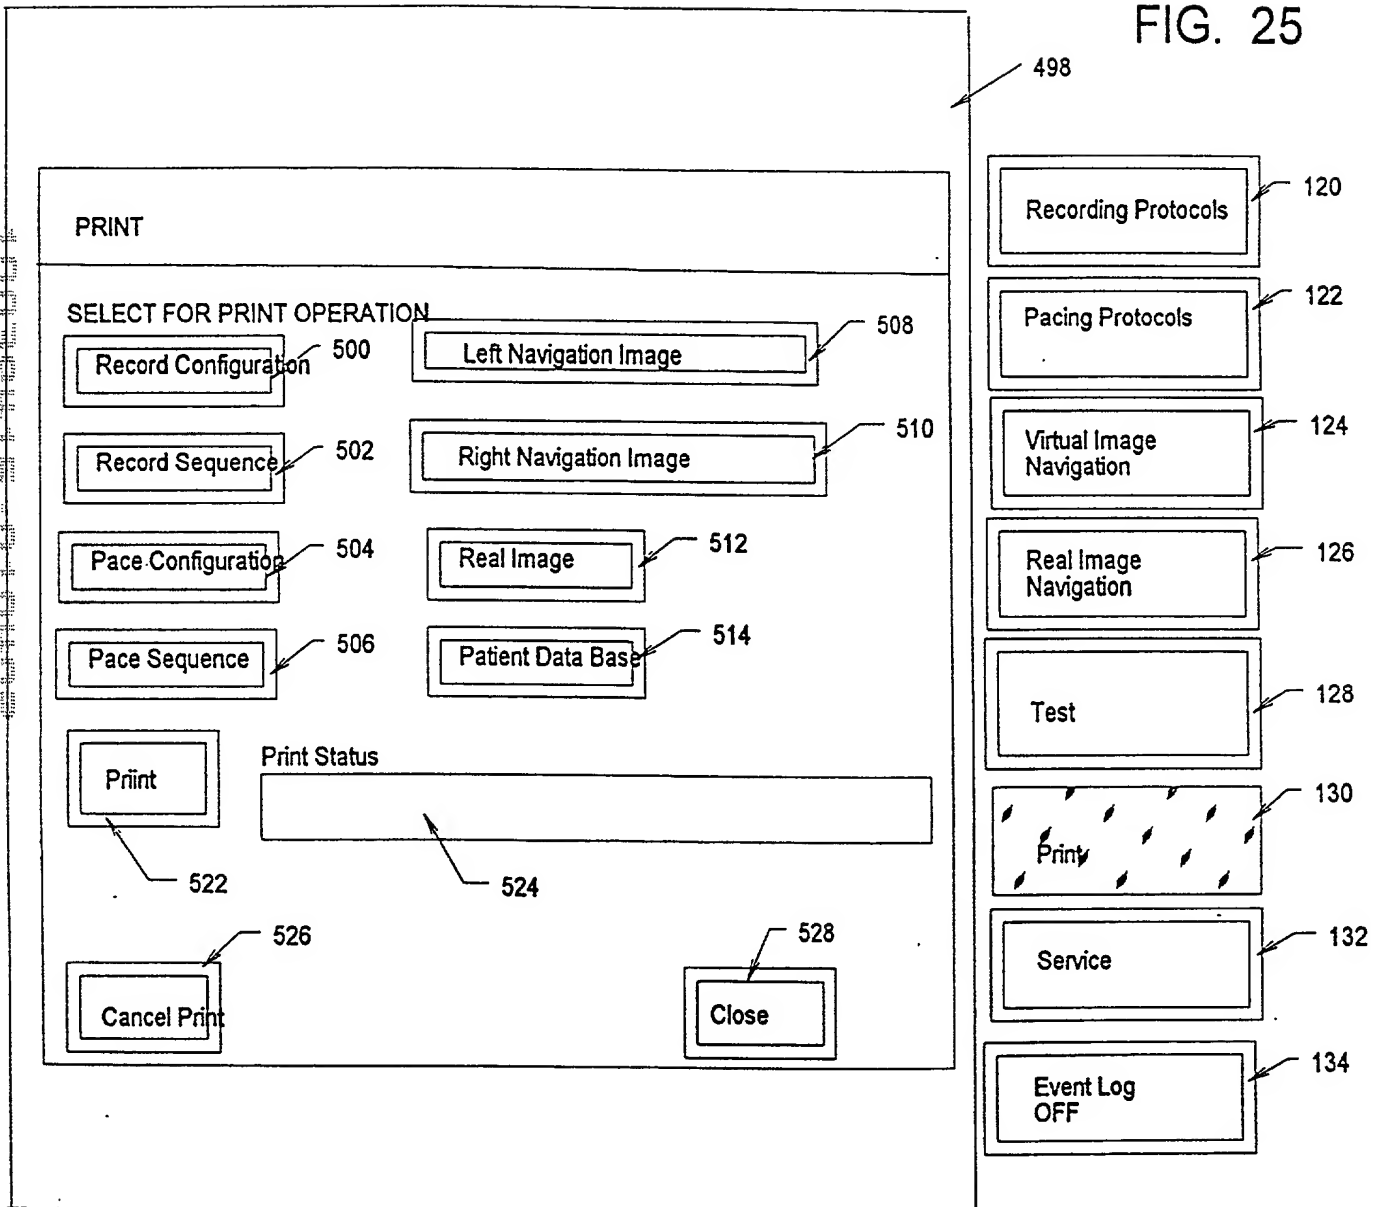


FIG. 26

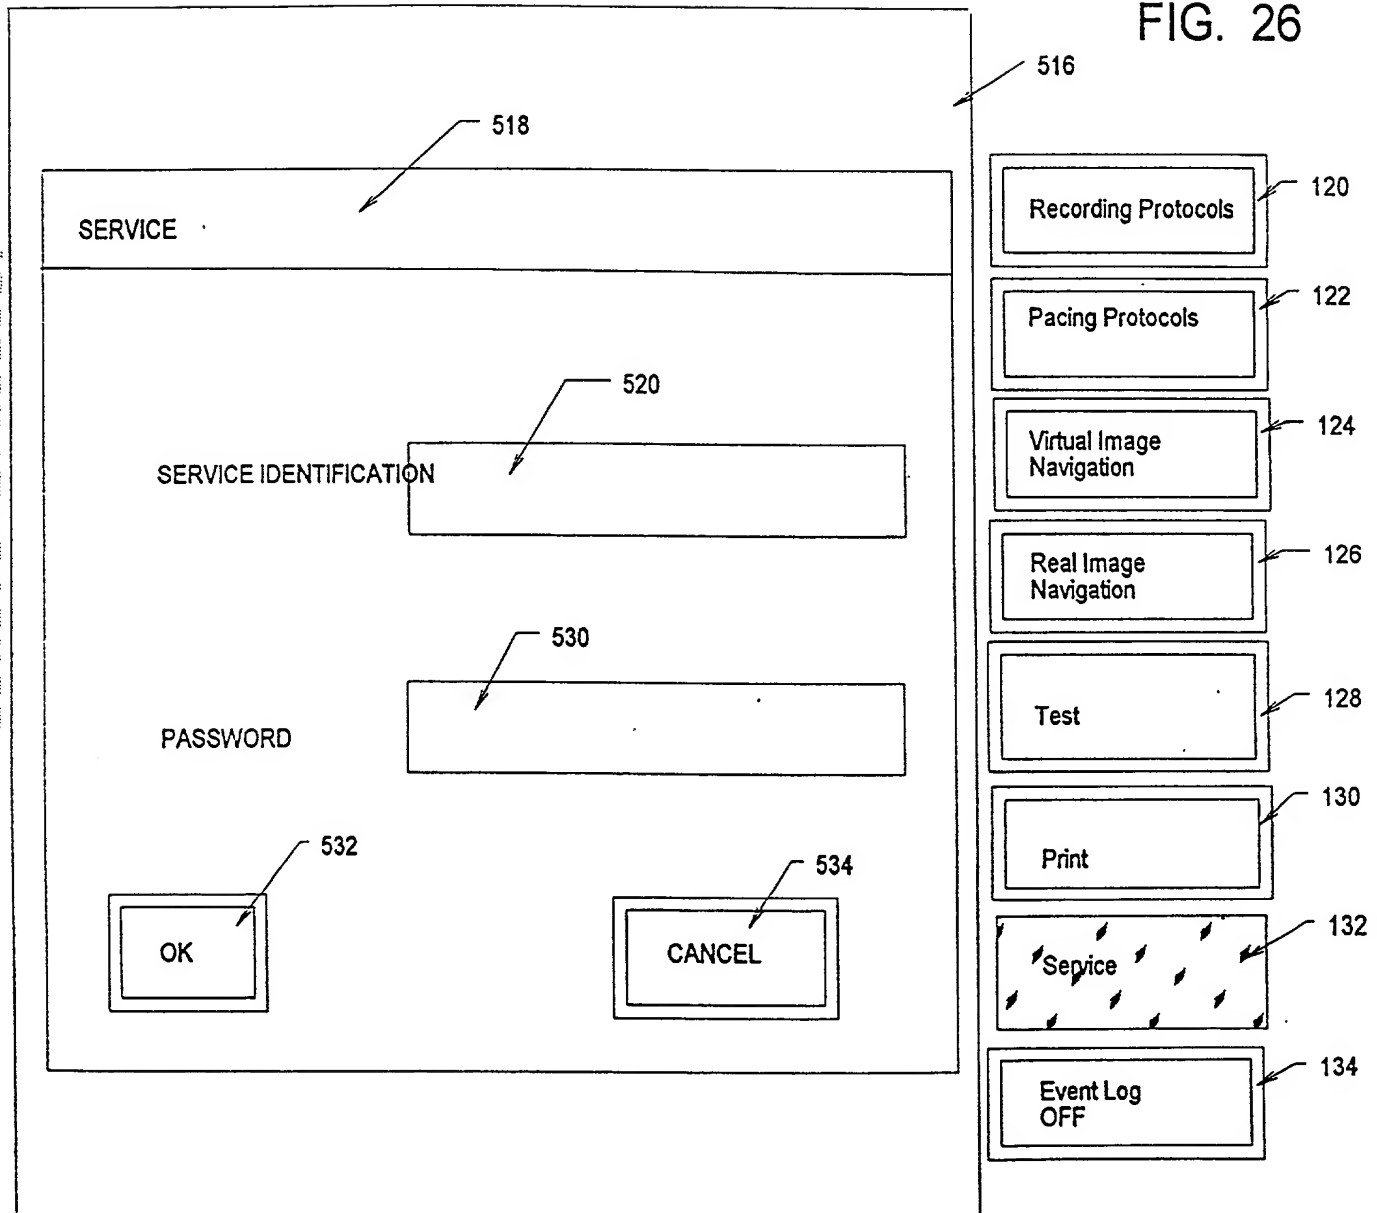


FIG. 27

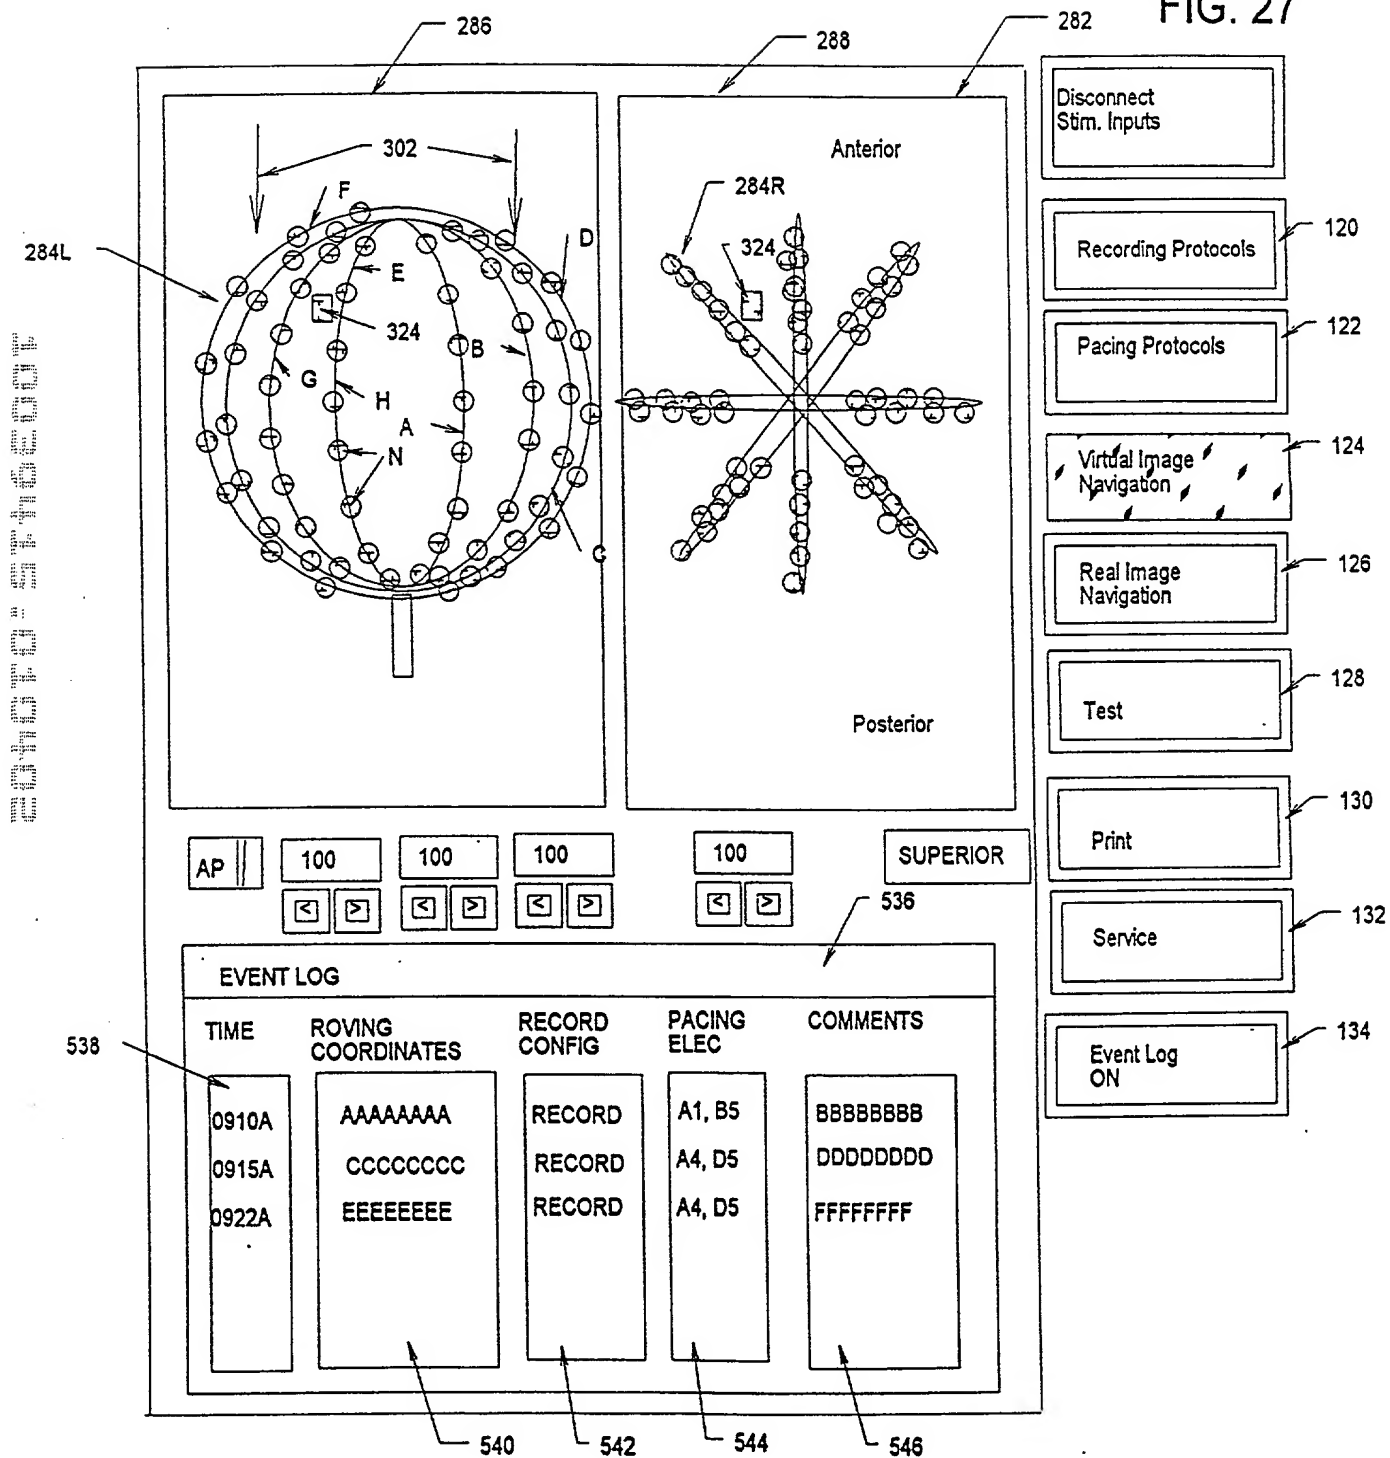


FIG. 28

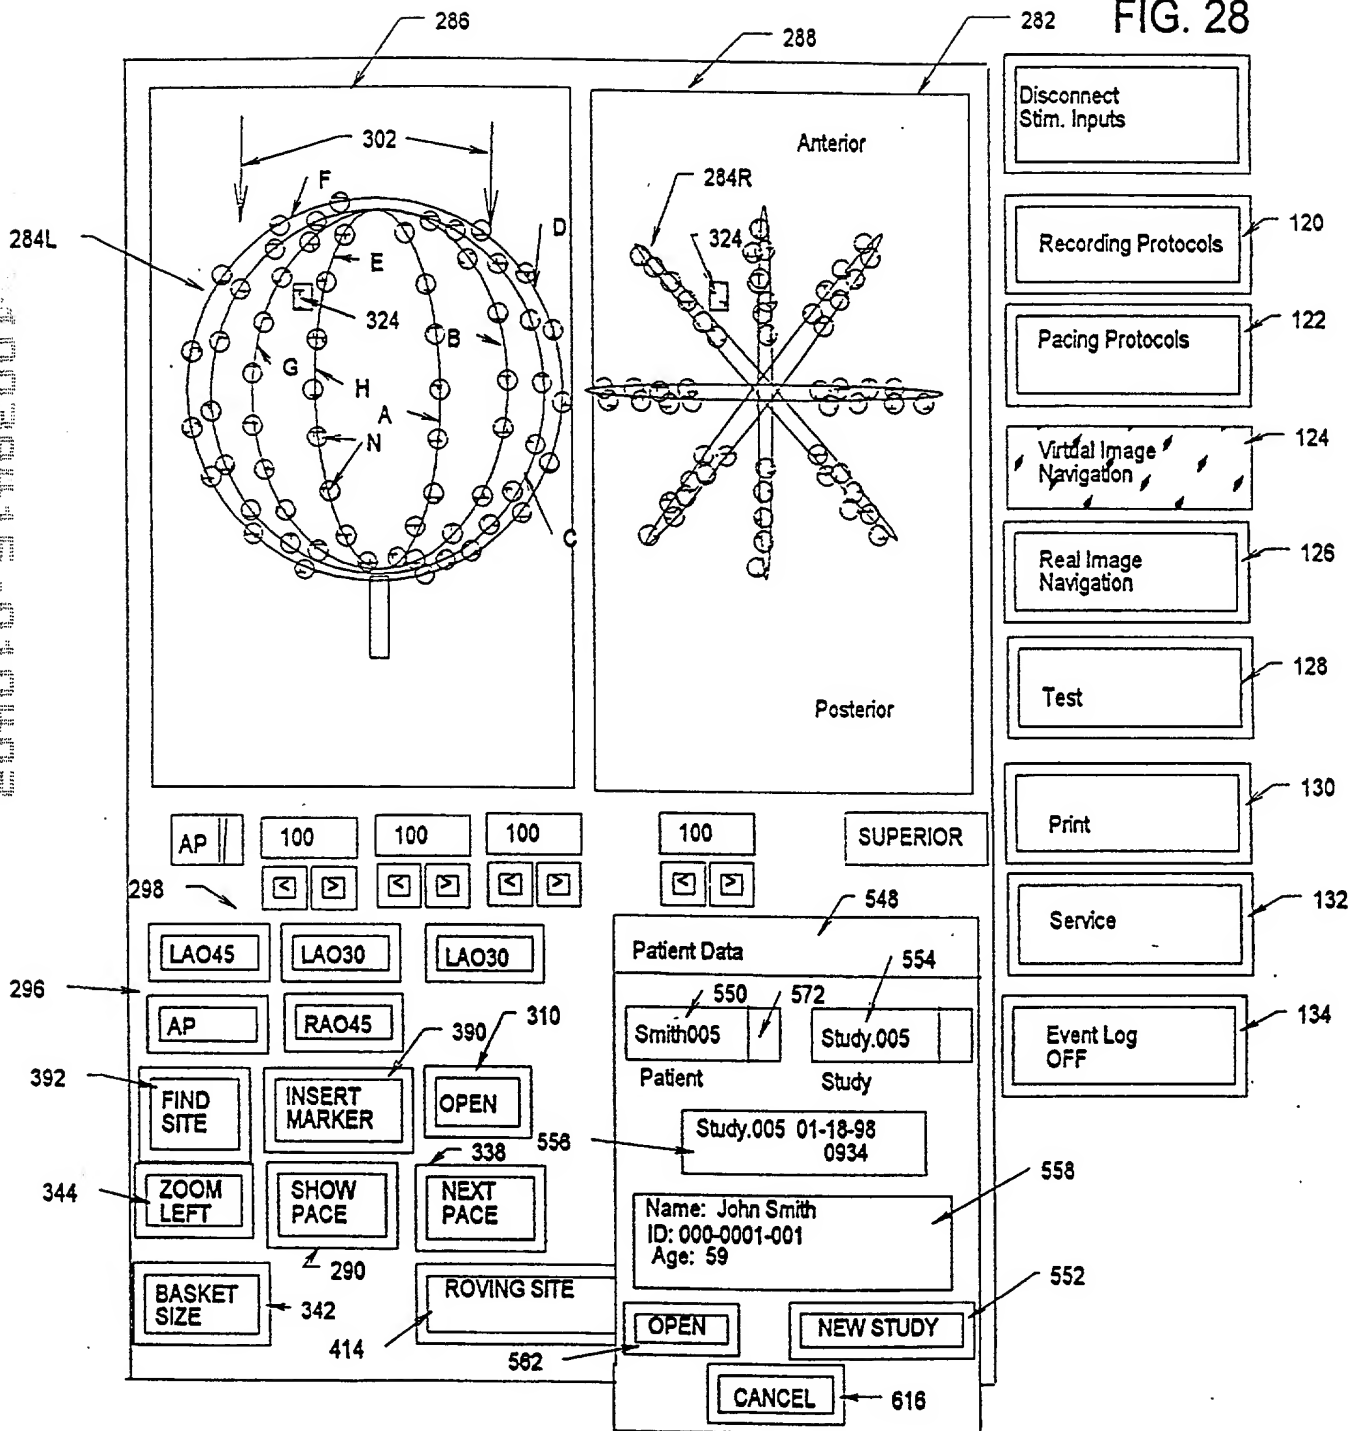


FIG. 29

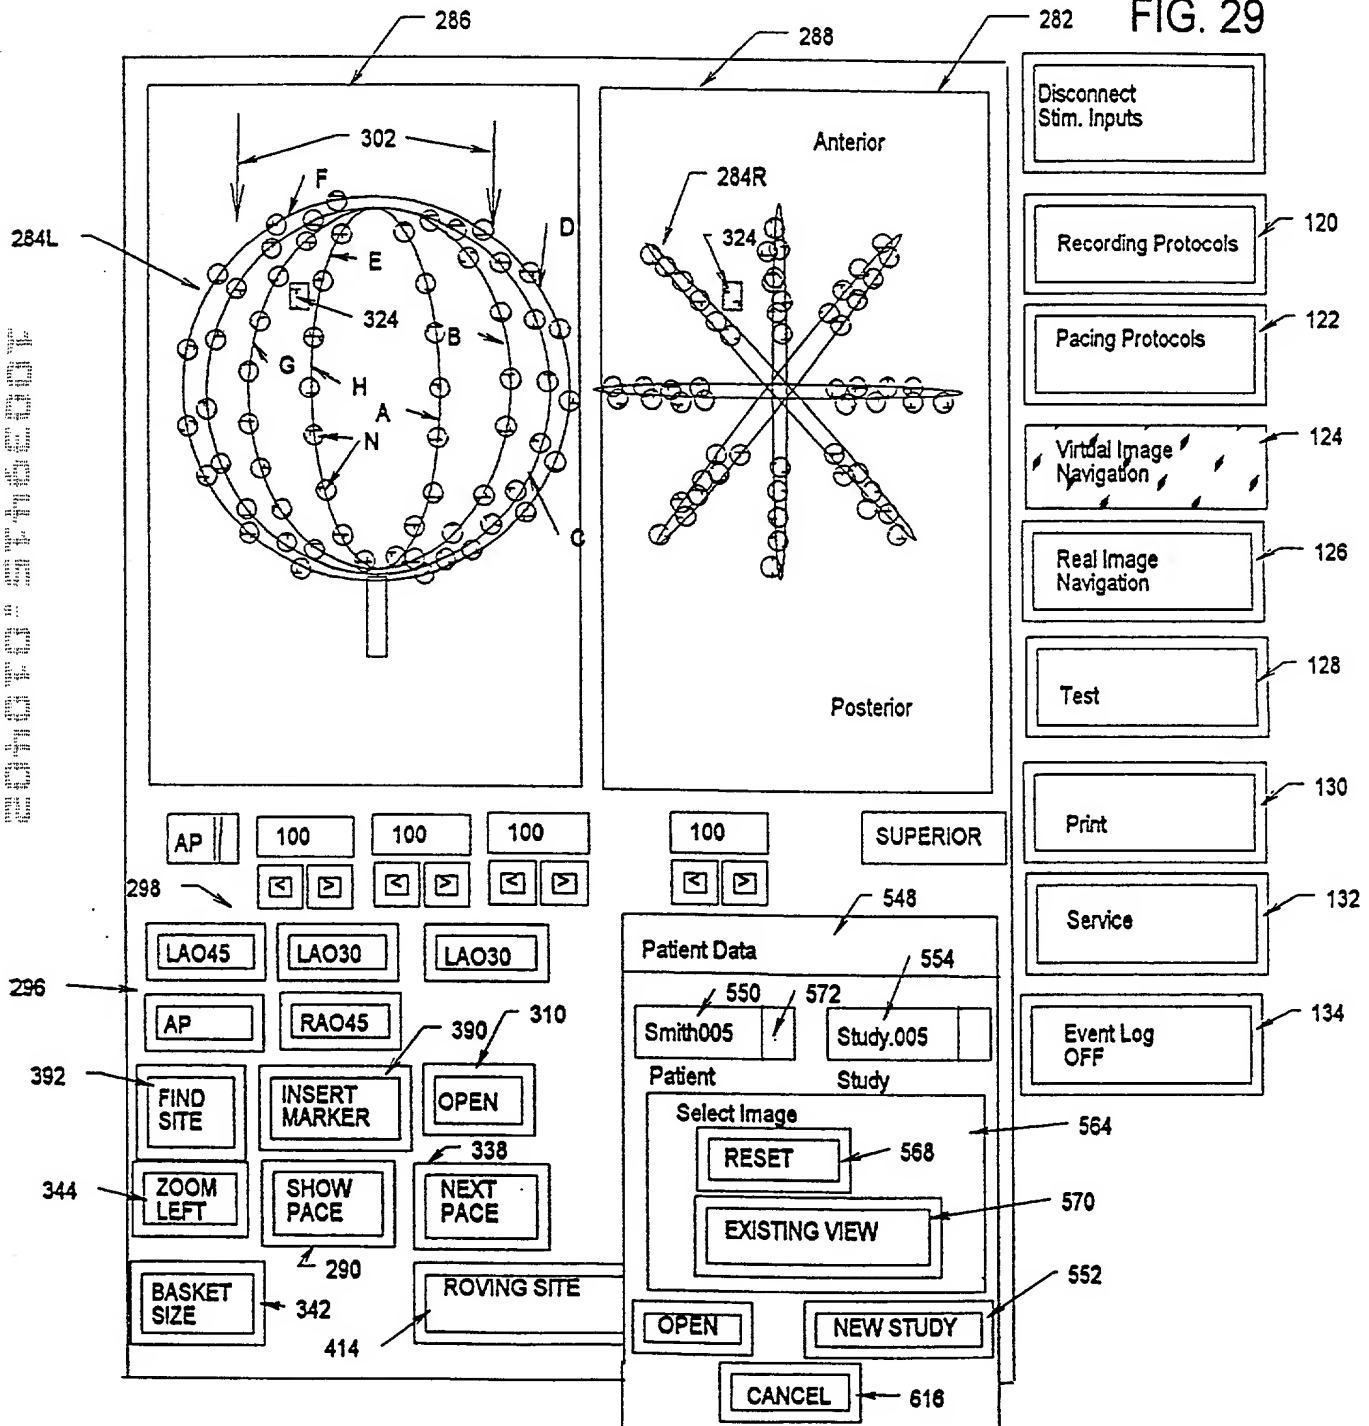


FIG. 30

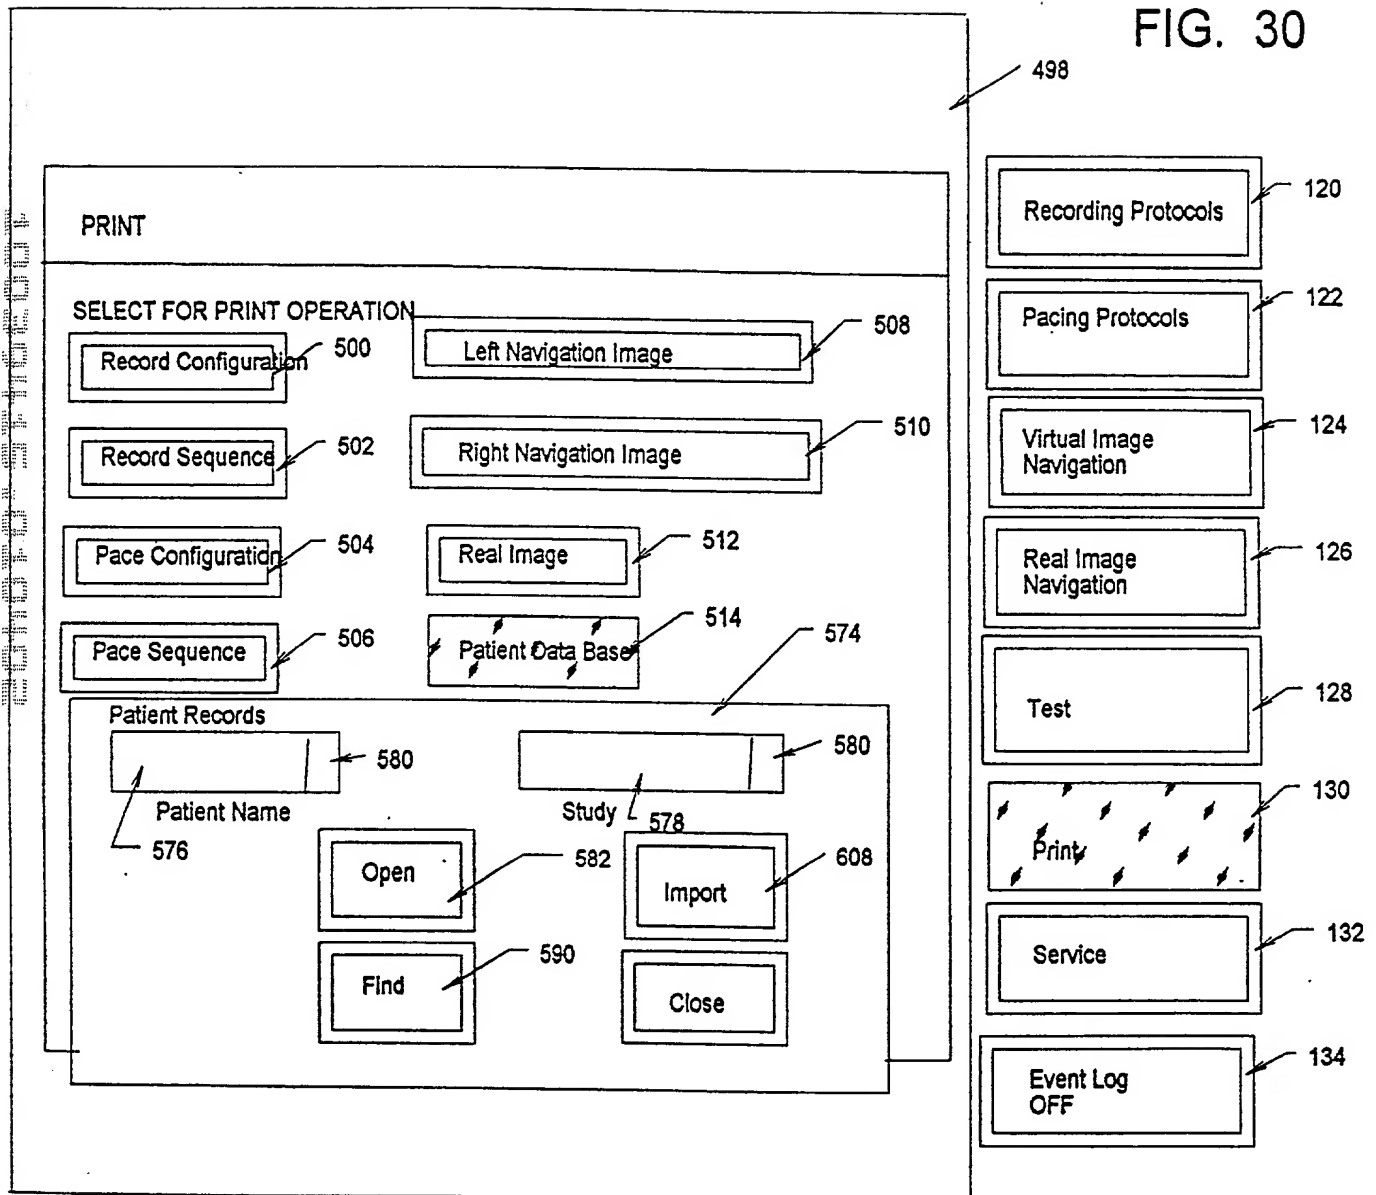


FIG. 31

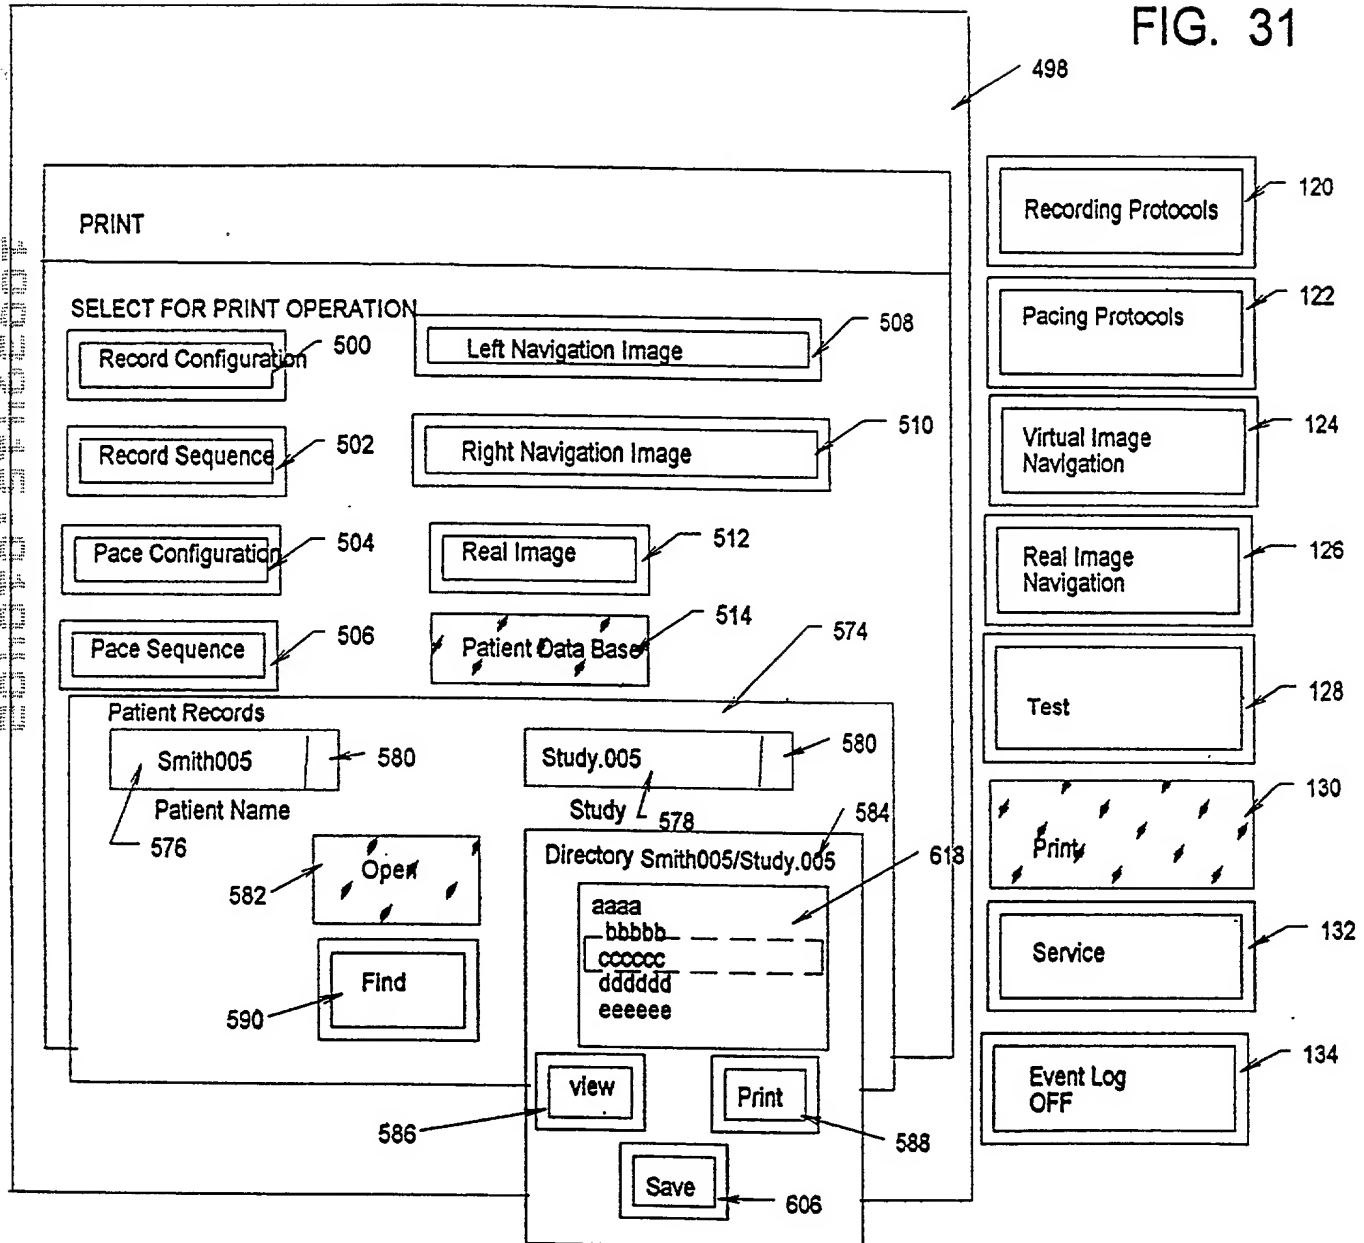


FIG. 32

